



Vodovodna 95
 1000 Ljubljana
 SLOVENIJA

T: +386 (0)1 428 44 93
 E: nfl@policija.si
www.policija.si

ANALYTICAL REPORT

2C-B-fly (C₁₂H₁₄BrNO₂)

2-{8-bromo-4,10-dioxatricyclo[7.3.0.03,7]dodeca-1,3(7),8-trien-2-yl}ethan-1-amine

Remark – other active cpd. detected: none

Sample ID:	1647-16
Sample description:	powder - white
Sample type:	RM-reference material
Comments ¹ :	Chiron AS Lot#17010; I-SEE project RM and report
Date of entry:	9/8/2016

Substance identified-structure ² (base form)	<p>The chemical structure shows a tricyclic core with a bromine atom (Br) at position 8. The core consists of a decalin system fused with a five-membered ring containing two oxygen atoms (ether linkages). A propylamino group (-NH₂) is attached to one of the ring carbons.</p>
Systematic name:	2-{8-bromo-4,10-dioxatricyclo[7.3.0.03,7]dodeca-1,3(7),8-trien-2-yl}ethan-1-amine
Other names:	2C-bromo-fly
Formula (per base form)	C ₁₂ H ₁₄ BrNO ₂
M _w (g/mol)	284.15
Salt form:	HCl
StdInChIKey	YZDFADGMVOSVIX-UHFFFAOYSA-N
Compound Class	Phenethylamines
Other active cpd. detected	none
Add.info (purity..)	98,0 %

¹ This report has been produced with the financial support of the Prevention of and fight against crime Programme of the European Union (grant agreement number JUST/2013/ISEC/DRUGS/AG/6426). The contents of this report are the sole responsibility of the National Forensic Laboratory and can in no way be taken to reflect the views of the European Commission.

² Created by OPSIN free tool: <http://opsin.ch.cam.ac.uk/> DOI: 10.1021/ci100384d



Report updates

date	comments (explanation)

Supporting information

Analytical technique:	applied	remarks
GC-MS (EI ionization)	+	NFL GC-RT (min): 8.19 BP(1): 254; BP(2): 256, BP(3) :115,
FTIR-ATR		
GC-IR (condensed phase)		

1. GC-MS (Agilent): GC-method is RT locked to tetracosane (9.258 min). Injection volume 1 ml and split mode (1:50). Injector temperature: 280 °C. Chromatographic separation: on column HP1-MS (100% dimethylpolysiloxane), length 30 m, internal diameter 0.25 mm, film thickness 0.25 µm. Carrier gas He: flow-rate 1.2 ml/min. GC oven program: 170 °C for 1 min, followed by heating up to 190 °C at rate 8 °C/min, then heating up to 293 °C at a rate of 18 °C/min, hold for 6.1 min, then heating at 50 °C/min up to 325 °C and finally 6.1 min isothermal. MSD source EI = 70 eV. GC-MS transfer line T= 235 °C, source and quadropole temperatures 280 °C and 180 °C, respectively. Scan range m/z scan range: from 50 (30 until 6 min.) to 550 (300 until 6 min) amu.

2. FTIR-ATR (Perkin Elmer): scan range 4000-400 cm⁻¹; resolution 4cm⁻¹

3. GC- (MS)-IR condensed phase (GC-MS (Agilent) & IR (Spectra analyses-Danny))


GC-method: Injection volume 1 ml and split mode (1:5). Injector temperature 280 °C. Chromatographic separation as above **(1)**. Split MS : IR = 1 : 9.

MSD source EI = 70 eV. GC-MS transfer line T= 235 °C, source and quadropole temperatures 280 °C and 180 °C, respectively. Scan range m/z scan range: from 50 (30 until 6 min.) to 550 (300) amu.

IR (condensed solid phase): IR scan range 4000 to 650, resolution 4 cm⁻¹.

FIGURES OF SPECTRA

MS (EI)

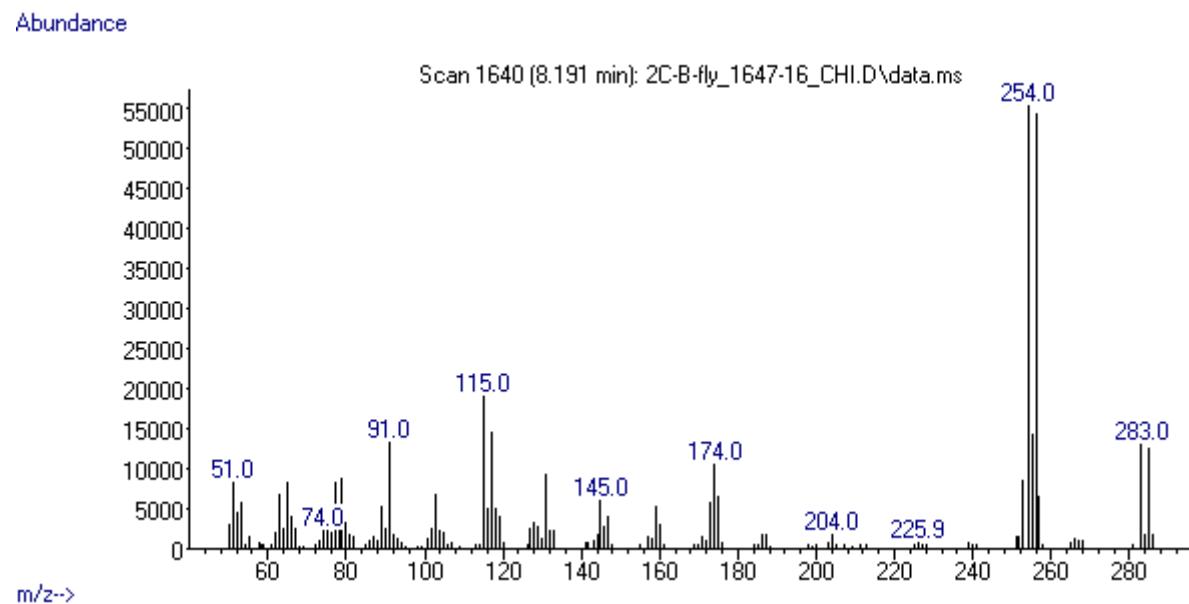

FTIR-ATR

