


ANALYTICAL REPORT

4-HO-MET (C₁₃H₁₈N₂O)

3-(2-(ethyl(methyl)amino)ethyl)-1H-indol-4-ol

Remark – other NPS detected: **none**

Sample ID:	1267-15
Sample description:	powder
Sample type:	test purchase /RESPONSE -purchasing
Date of entry (DD/MM/YYYY) into NFL database:	02/09/2015
Report updates (if any) will be published here:	http://www.policija.si/apps/nfl_response_web/seznam.php

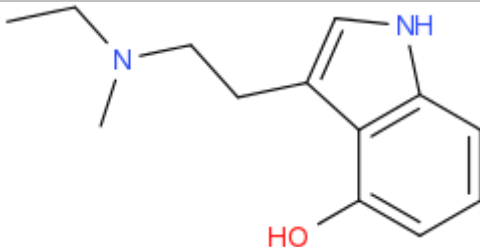Substance identified - structure ¹ (base form)	
Systematic name	3-(2-(ethyl(methyl)amino)ethyl)-1H-indol-4-ol
Other names	4-hydroxy-N-methyl-N-ethyltryptamine
Formula (per base form)	C ₁₃ H ₁₈ N ₂ O
M _w (g/mol)	218,3
Salt form/anions detected	fumarate
StdInChIKey (per base form)	ORWQBKPSGDRPPA-UHFFFAOYSA-N
Other NPS detected	none
Additional info (purity..)	substantial amount of fumaric acid-TMS derivative proved by GC-MS, fumaric anions by IC

¹ Created by OPSIN free tool: <http://opsin.ch.cam.ac.uk/> DOI: 10.1021/ci100384d

Report updates

date	comments (explanation)
04/09/2025	Common name changed from 4-OH-MET-fumarate to 4-HO-MET-fumarate

Instrumental methods (if applied) in NFL

1. GC-MS (Agilent): GC-method is RT locked to tetracosane (9.258 min). Injection volume 1 µl and split mode (1:50). Injector temperature: 280 °C. Chromatographic separation: on column HP1-MS (100% dimethylpolysiloxane), length 30 m, internal diameter 0.25 mm, film thickness 0.25 µm. Carrier gas He: flow-rate 1.2 ml/min. GC oven program: 170 °C for 1 min, followed by heating up to 190 °C at rate 8 °C/min, then heating up to 293 °C at a rate of 18 °C/min, hold for 6.1 min, then heating at 50 °C/min up to 325 °C and finally 9.1 min isothermal. MSD source EI = 70 eV. GC-MS transfer line T= 235°C, source and quadropole temperatures 280°C and 180°C, respectively. Scan range m/z scan range: from 50 (30 until 6 min.) to 550 (300 until 6 min) amu.

2. HPLC-TOF (Agilent): 6230B TOF with Agilent 1260 Infinity HPLC with binary pump, column: Zorbax Eclipse XDB-C18, 50 x 4.6 mm, 1.8 micron. Mobile phases (A) 0.1% formic acid and 1mM ammonium formate in water; (B) 0.1% formic acid in methanol (B). Gradient: starting at 5% B, changing to 40% B over 4 min, then to 70% over 2 min and in 5 min to 100%, hold 1 min and back to 5%, equilibration for 1.7 min. The flow rate: 1.0 ml/min; Injection volume 1 µl. MS parameters: 2GHz, Extended Dynamic range mode to a maximum of 1700 amu, acquisition rate 1.30 spectra/sec. Sample ionisation: by Agilent Jet Stream technology (Dual AJS ESI). Ion source: positive ion scan mode with mass scanning from 82 to 1000 amu. Other TOF parameters: drying gas (N₂) and sheath temperature 325 °C; drying gas flow rate 6 l/min; sheath gas flow rate 8 l/min; nebulizer 25 psig; Vcap. 4000 V; nozzle 2000 V; skimmer 65 V; fragmentor 175 V and Octopole RF 750 V.

3. FTIR-ATR (Perkin Elmer): scan range 4000-400 cm⁻¹; resolution 4cm⁻¹

4. GC- (MS)-IR solid phase (GC-MS (Agilent) & IR (Spectra analyses-Danny)

GC-method: Injection volume 1 µl and split mode (1:5). Injector temperature 280 °C. Chromatographic separation as above **(1)**. Split MS : IR = 1: 9.

MSD source EI = 70 eV. GC-MS transfer line T= 235°C, source and quadropole temperatures 280°C and 180°C, respectively. Scan range m/z scan range: from 50 (30 until 6 min.) to 550 (300) amu.

IR (condensed (solid) phase): IR scan range 4000 to 650, resolution 4 cm⁻¹.

5. IC (anions) (Thermo Scientific, Dionex ICS 2100), Column: IonPac AS19, 2 x 250mm; Eluent: 10mM KOH from 0 to 10 min, 10-58 mM from 10 to 40min; Flow rate: 0.25 ml/min; Temperature: 30°C; Suppressor: AERS 500 2mm, suppressor current 13mA; Inj. Volume: 25 µl

Supporting information


Solubility in	result/remark
CH ₂ Cl ₂	soluble
MeOH	soluble
H ₂ O	soluble

Analytical technique:	applied	remarks
GC-MS (EI ionization)	+	NFL GC-RT (min): 7,51 BP(1): 72; BP(2): 218,BP(3) :146,
HPLC-TOF	+	Exact mass (theoretical): 218,1419; measured value Δppm:-1,55; formula:C13H18N2O
FTIR-ATR	+	direct measurement (sample as received)
FTIR (solid phase) always as base form	+	
IC (anions)	+	
NMR (in FKKT)	+	
validation		MS consistent with the one from ENFSI 2015 lib
other		


ANALYTICAL RESULTS

MS (EI)


Abundance

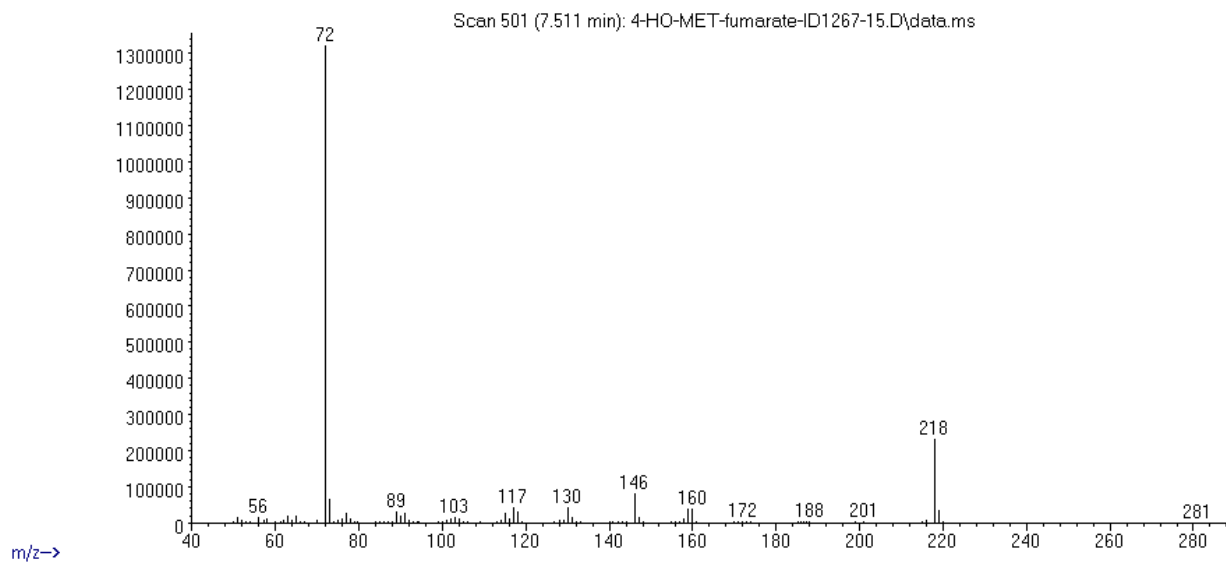

FTIR-ATR - direct measurement (sample as received)

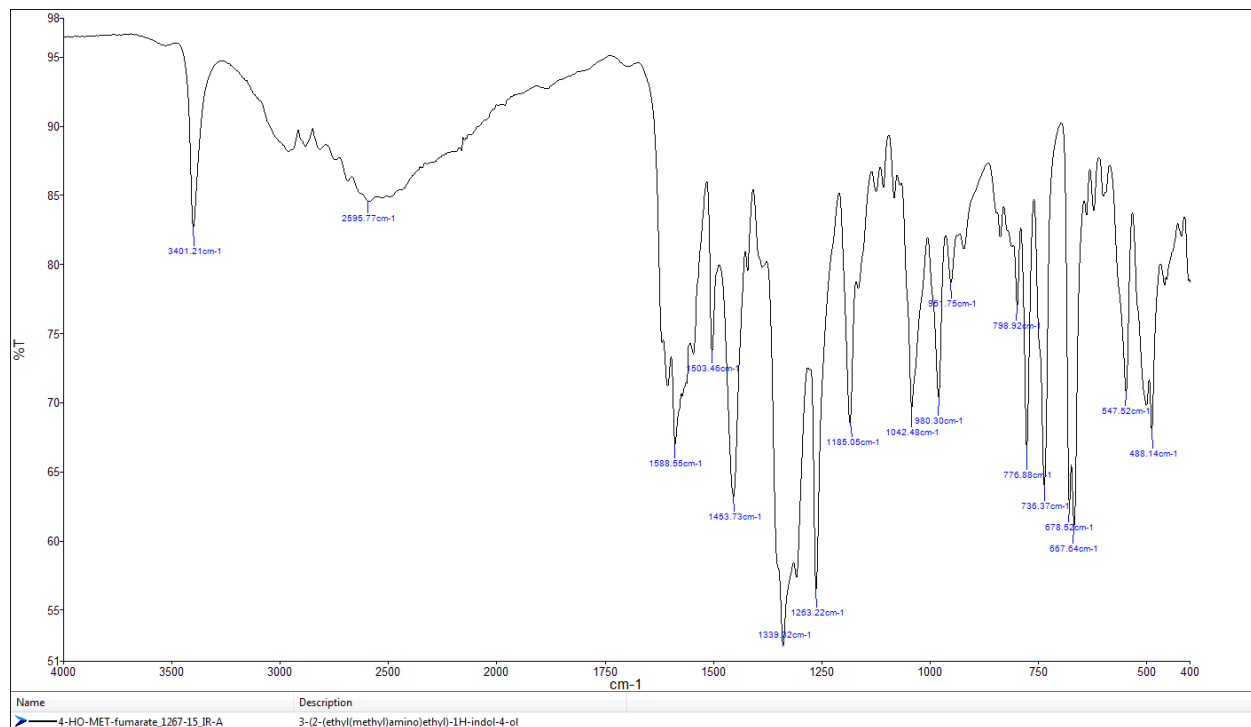

IR (solid phase – after chromatographic separation)

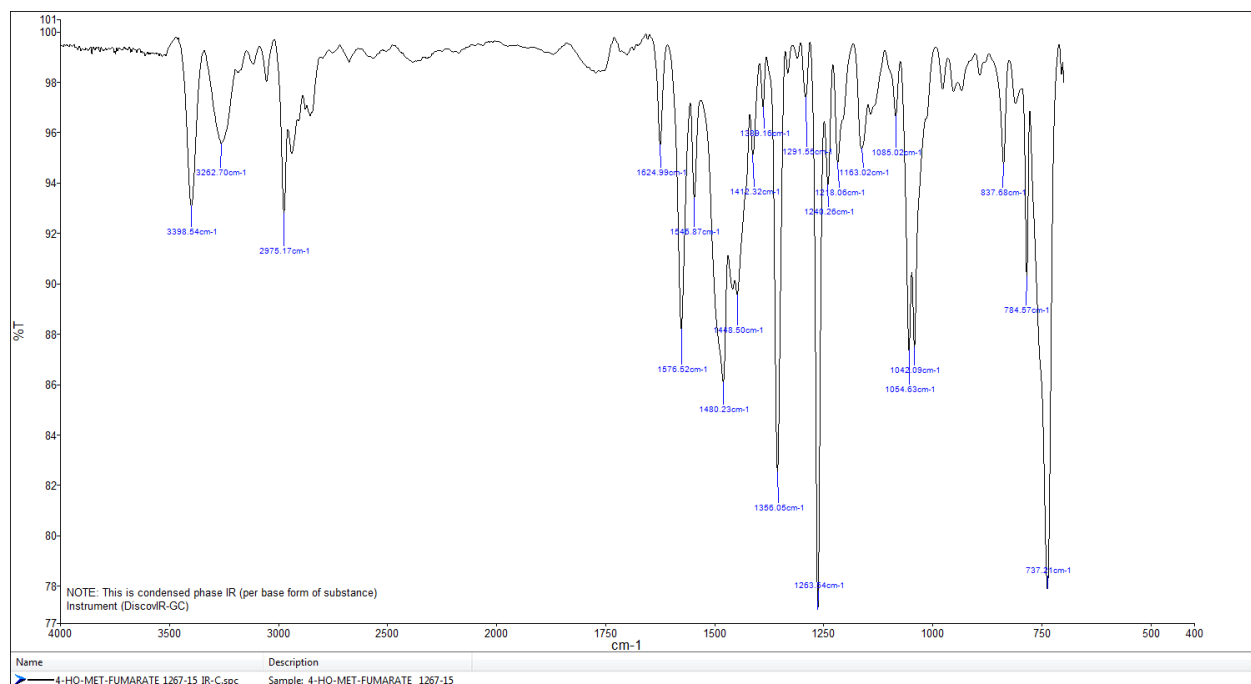

Target Compound Screening Report



Data File	4-HO-MET-fumarate_1267-15_TOF.d	Sample Name	1267-15
Sample Type	Sample	Position	P1-C6
Instrument Name	6230B TOF LC-MS	User Name	TG
Acq Method	droge general-13-5-2015-XDB-C18-ESI-poz.m	Acquired Time	9/2/2015 4:33:50 PM
IRM Calibration Status	Success	DA Method	Droge_Default.m
Comment	extract in MeOH		

Compound Table


Label	Tgt Name	Obs. RT	Obs. Mass
Cpd 2: 4-HO-MET (fumarate)	4-HO-MET (fumarate)	3.258	218.1422

Name	Obs. m/z	Obs. RT	Obs. Mass	DB RT	DB Formula	DB Mass	DB Mass Error (ppm)	Find Cpd Algorithm
4-HO-MET (fumarate)	219.1495	3.258	218.1422	3.25	C13 H18 N2 O	218.1419	-1.55	Find by Molecular Feature

Compound Chromatograms

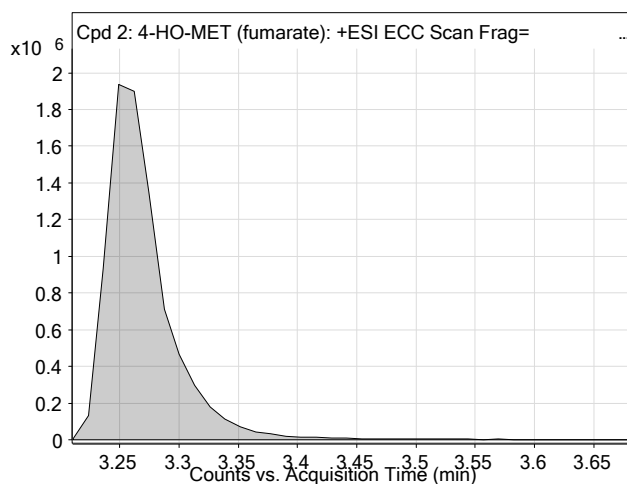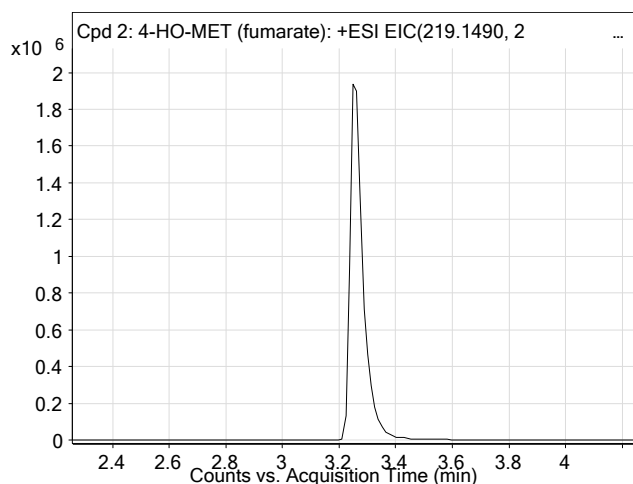

MFE MS Zoomed Spectrum

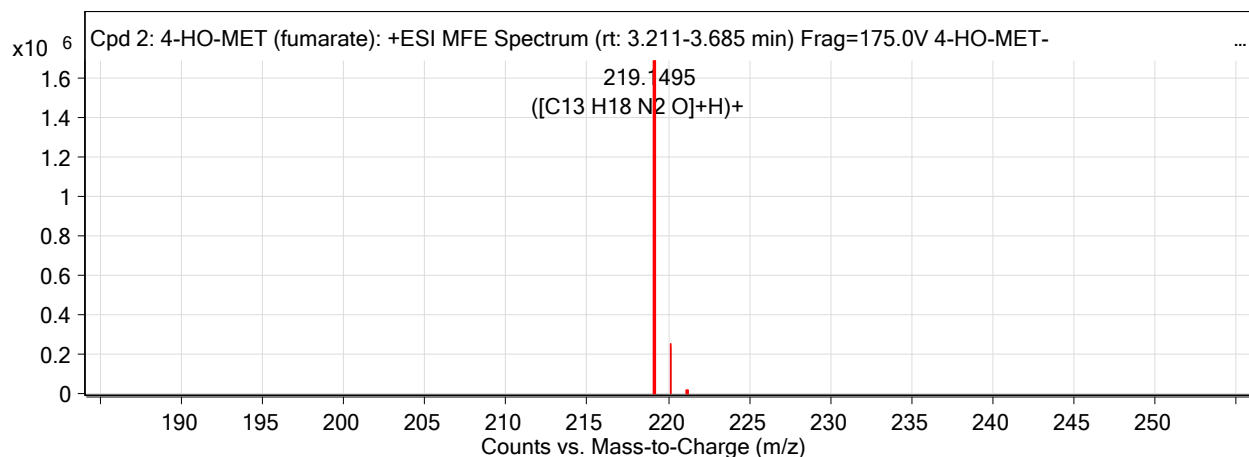


MS Spectrum Peak List

Obs. m/z	Charge	Abund	Formula	Ion/Isotope
219.1495	1	1685499.5	C13 H18 N2 O	(M+H)+
220.1526	1	236058.54	C13 H18 N2 O	(M+H)+
221.1552	1	19894.21	C13 H18 N2 O	(M+H)+

MS Zoomed Spectrum

Target Compound Screening Report

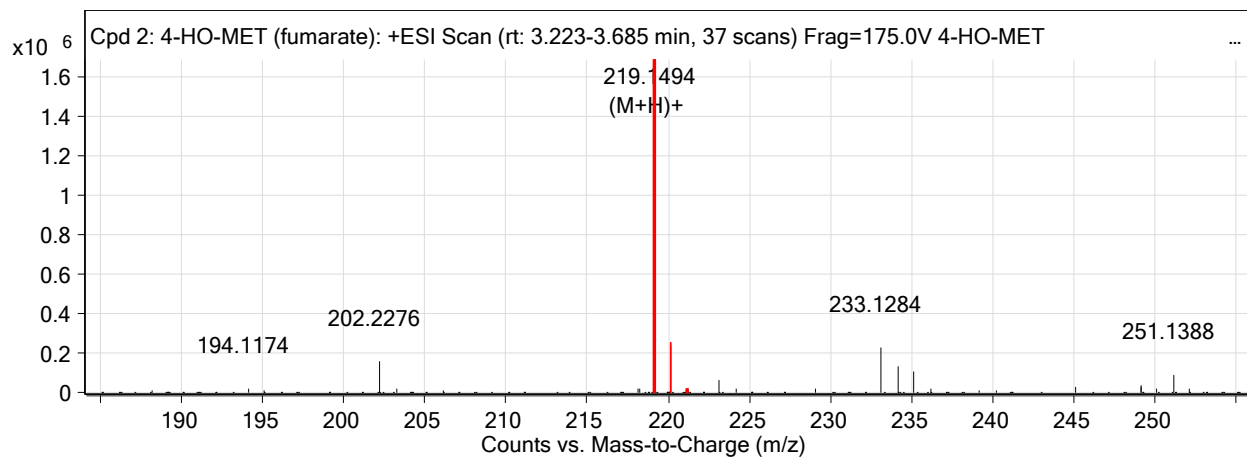


--- End Of Report ---

Peak Integration Report


Sample Name:	4-HO-MET_1267-15_IC	Inj. Vol.:	25,00
Injection Type:	Unknown	Dilution Factor:	1,0000
Program:	ANIONI	Operator:	kemija
Inj. Date / Time:	21-okt-2015 / 21:35	Run Time:	42,00

No.	Time min	Peak Name	Peak Type	Area $\mu\text{S}\cdot\text{min}$	Height μS	Amount mg/L
1,00	31,05	Fumarate	BMB	2,98	8,91	n.a.
		TOTAL:		2,98	8,91	0,00

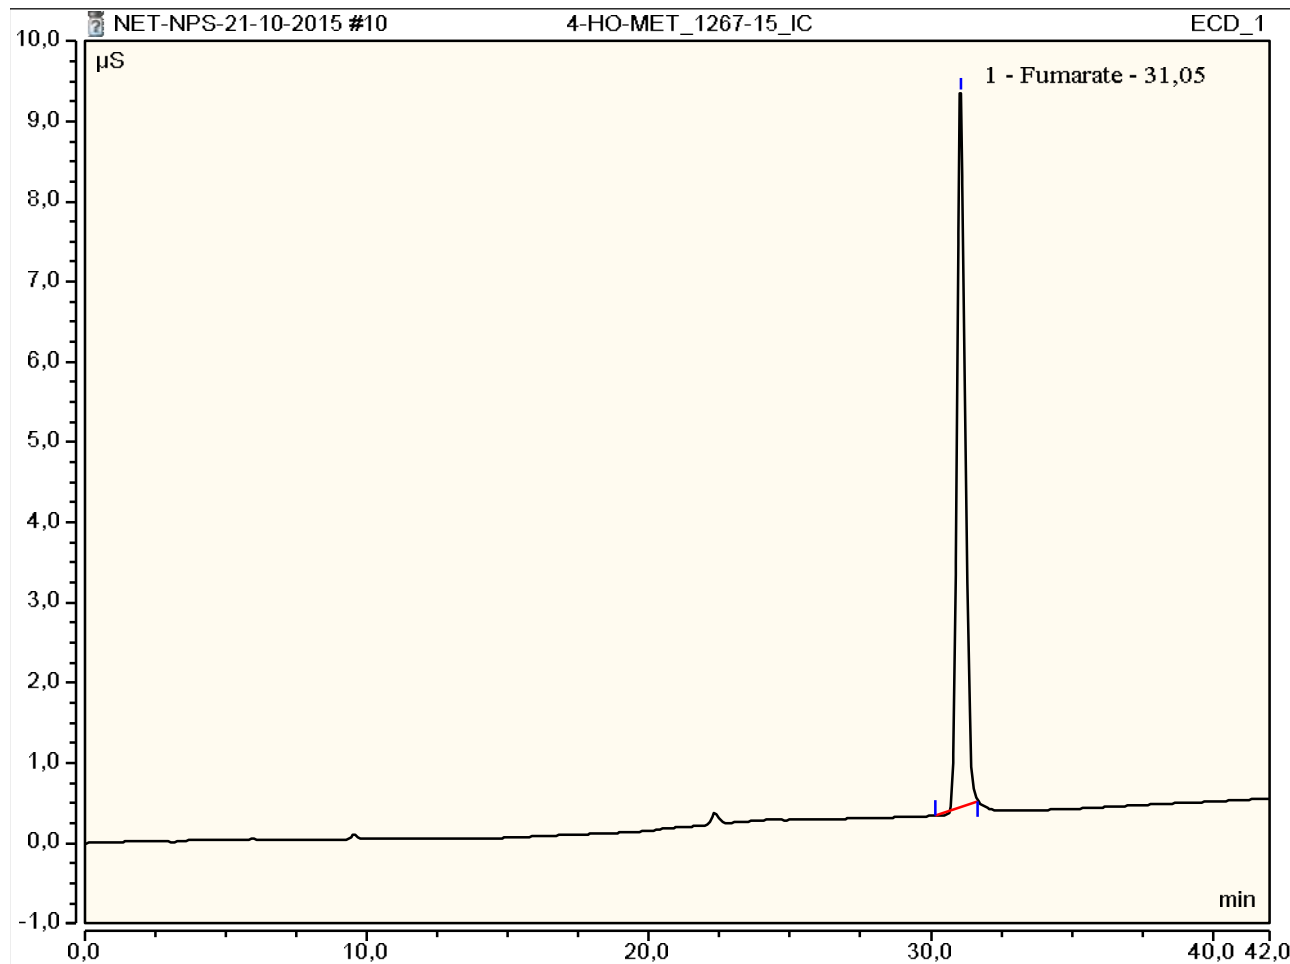



REPORT

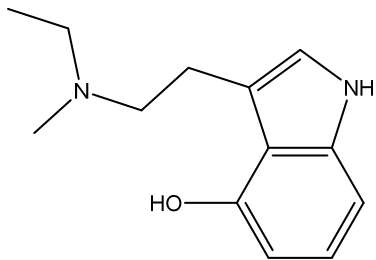Sample ID:	1267-15
Our notebook code:	P-1267-15
NMR sample preparation:	15 mg dissolved in 0.7 mL DMSO- <i>d</i> ₆
NMR experiments:	¹ H, ¹³ C, ¹ H- ¹ H <i>gs</i> -COSY, ¹ H- ¹³ C <i>gs</i> -HSQC.
Proposed structure:	
Chemical name:	3-(2-(ethyl(methyl)amino)ethyl)-1H-indol-4-ol
Comments:	- Structure elucidation based on 1D and 2D NMR spectra - Compound is not pure by NMR, it contains organic impurities, probably two different compounds (signals in ¹³C NMR at 168.6, 135.7, 45.5 and 9.8; signals in ¹H NMR at 2.8 and 1.1).
Supporting information:	Copies of ¹ H and ¹³ C NMR spectra
Author:	Prof. Dr. Janez Košmrlj, Doc. Dr. Krištof Kranjc
Date of report:	November 17, 2015

```
Current Data Parameters
NAME                P-1267-15
EXPNO                1
PROCNO              1
```

```

F2 - Acquisition Parameters
Date_      20151101
Time       6.20
INSTRUM    spect
PROBHD     5 mm PABBO BB-
PULPROG    zg30
TD          65536
SOLVENT    DMSO
NS          16
DS          2
SWH         10330.578 Hz
FIDRES     0.157632 Hz
AQ          3.1719923 sec
RG          80.6
DW          48.400 usec
DE          6.50 usec
TE          296.0 K
D1          1.0000000 sec

```

```
===== CHANNEL f1 =====
NUC1                1H
P1                  8.90 usec
PLW1                26.0000000 W
SFO1                500.1330885 MHz
```

```
F2 - Processing parameters
SI                65536
SF                500.1300051 MHz
WDW               EM
SSB               0
LB                0.30 Hz
GB               0
PC                1.00
```

P-1267-15

168.57
152.09
139.18
135.67
122.45
121.86
117.15
111.82
103.84
103.28
57.85
50.62
45.54
40.65
23.29
10.82
9.78

180 160 140 120 100 80 60 40 20 ppm

```
Current Data Parameters
NAME          P-1267-15
EXPNO          4
PROCNO         1
```

```

F2 - Acquisition Parameters
Date_      20151101
Time       9.47
INSTRUM    spect
PROBHD     5 mm PABBO BB-
PULPROG    zgpg30
TD          65536
SOLVENT     DMSO
NS          5120
DS          4
SWH         29761.904 Hz
FIDRES     0.454131 Hz
AQ          1.1010548 sec
RG          2050
DW          16.800 usec
DE          6.50 usec
TE          296.0 K
D1          1.00000000 sec
D11         0.03000000 sec

```

```
===== CHANNEL f1 =====
NUC1                13C
P1                   9.00 usec
PLW1                122.00000000 W
SFO1                125.7703637 MHz
```

```
===== CHANNEL f2 =====
CPDPRG2          waltz16
NUC2              1H
PCPD2            80.00 usec
PLW2             26.00000000 W
PLW12            0.32179001 W
PLW13            0.20595001 W
SFO2             500.1320005 MHz
```

```

F2 - Processing parameters
SI                      32768
SF                      125.7577890 MHz
WDW                      EM
SSB                      0
LB                      1.00 Hz
GB                      0
PC                      1.40

```