



Vodovodna 95
1000 Ljubljana
SLOVENIJA

T: +386 (0)1 428 44 93
E: nfl@policija.si
www.policija.si


ANALYTICAL REPORT

5CI-THJ-018 (C23H21CIN2O)

1-(5-chloropentyl)-3-(naphthalene-1-carbonyl)-1H-indazole

Remark – other active cpd. detected: none

| | |
|-------------------------|---|
| Sample ID: | 1774-17 |
| Sample description: | liquid - transparent |
| Sample type: | RM-reference material |
| Comments ¹ : | CAY Lot#0487612-5; RESPONSE -purchasing |
| Date of entry: | 3/9/2017 |
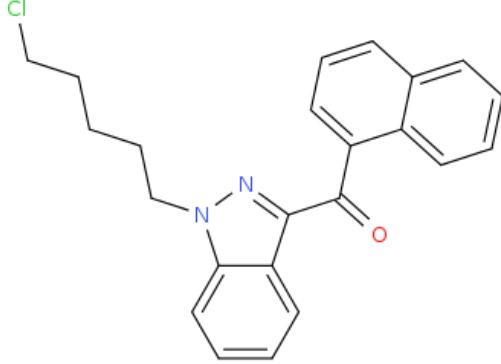
| | |
|---|---|
| Substance identified-structure ² (base form) |  |
| Systematic name: | 1-(5-chloropentyl)-3-(naphthalene-1-carbonyl)-1H-indazole |
| Other names: | 5-chloropentyl JWH 018 indazole analog; THJ 018 chloro analog; (1-(5-chloropentyl)-1H-indazol-3-yl)(naphthalen-1-yl)methanone |
| Formula (per base form) | C23H21CIN2O |
| M _w (g/mol) | 376,88 |
| Salt form: | base |
| StdInChIKey (for base form) | KLRDJQQYGMTILS-UHFFFAOYSA-N |
| Other active cpd. detected | none |
| Add.info (purity..) | purity 98%; 10mg/ml ACN solution |

¹ This report has been produced with the financial support of the Prevention of and fight against crime Programme of the European Union (grant agreement number JUST/2013/ISEC/DRUGS/AG/6413). The contents of this report are the sole responsibility of the National Forensic Laboratory and can in no way be taken to reflect the views of the European Commission.

² Created by OPSIN free tool: <http://opsin.ch.cam.ac.uk/> DOI: 10.1021/ci100384d



Report updates

| date | comments (explanation) |
|------|------------------------|
| | |
| | |
| | |
| | |

Supporting information

| Analytical technique: | applied | remarks |
|-------------------------|---------|---|
| GC-MS (EI ionization) | + | NFL GC-RT (min): 16,13 BP(1): 127; BP(2): 271,BP(3) :375, |
| FTIR-ATR | + | solvent removed |
| GC-IR (condensed phase) | + | always as base form |

1. GC-MS (Agilent): GC-method is RT locked to tetracosane (9.258 min). Injection volume 1 ml and split mode (1:50). Injector temperature: 280 °C. Chromatographic separation: on column HP1-MS (100% dimethylpolysiloxane), length 30 m, internal diameter 0.25 mm, film thickness 0.25 µm. Carrier gas He: flow-rate 1.2 ml/min. GC oven program: 170 °C for 1 min, followed by heating up to 190 °C at rate 8 °C/min, then heating up to 293 °C at a rate of 18 °C/min, hold for 7.1 min, then heating at 50 °C/min up to 325 °C and finally 6.1 min isothermal. MSD source EI = 70 eV. GC-MS transfer line T= 235 °C, source and quadropole temperatures 280 °C and 180 °C, respectively. Scan range m/z scan range: from 50 (30 until 6 min.) to 550 (300 until 6 min) amu.

2. FTIR-ATR (Perkin Elmer): scan range 4000-400 cm⁻¹; resolution 4cm⁻¹

3. GC- (MS)-IR condensed phase (GC-MS (Agilent) & IR (Spectra analyses-Danny))

GC-method: Injection volume 1 ml and split mode (1:5). Injector temperature 280 °C. Chromatographic separation as above **(1)**. Split MS : IR = 1 : 9.

MSD source EI = 70 eV. GC-MS transfer line T= 235 °C, source and quadropole temperatures 280 °C and 180 °C, respectively. Scan range m/z scan range: from 50 (30 until 6 min.) to 550 (300) amu.


IR (condensed (solid) phase): IR scan range 4000 to 650, resolution 4 cm⁻¹.

4. HPLC-TOF for exact monoisotopic mass and empirical formula control - results are not shown in the report.


ANALYTICAL RESULTS

MS (EI)

Abundance

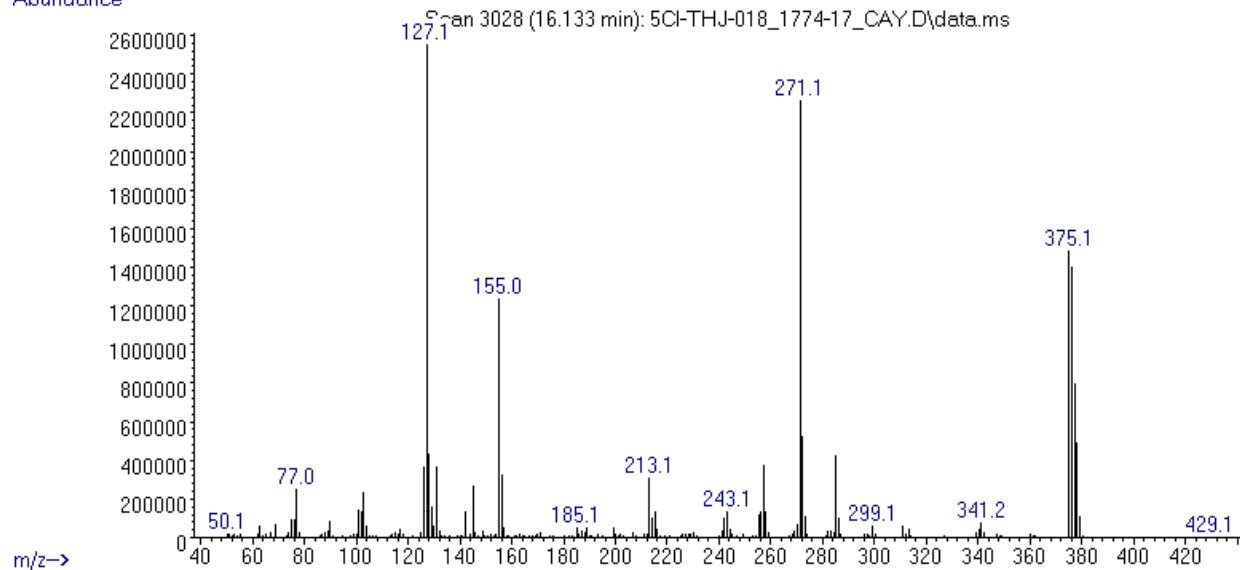

FTIR-ATR - (solvent evaporated)

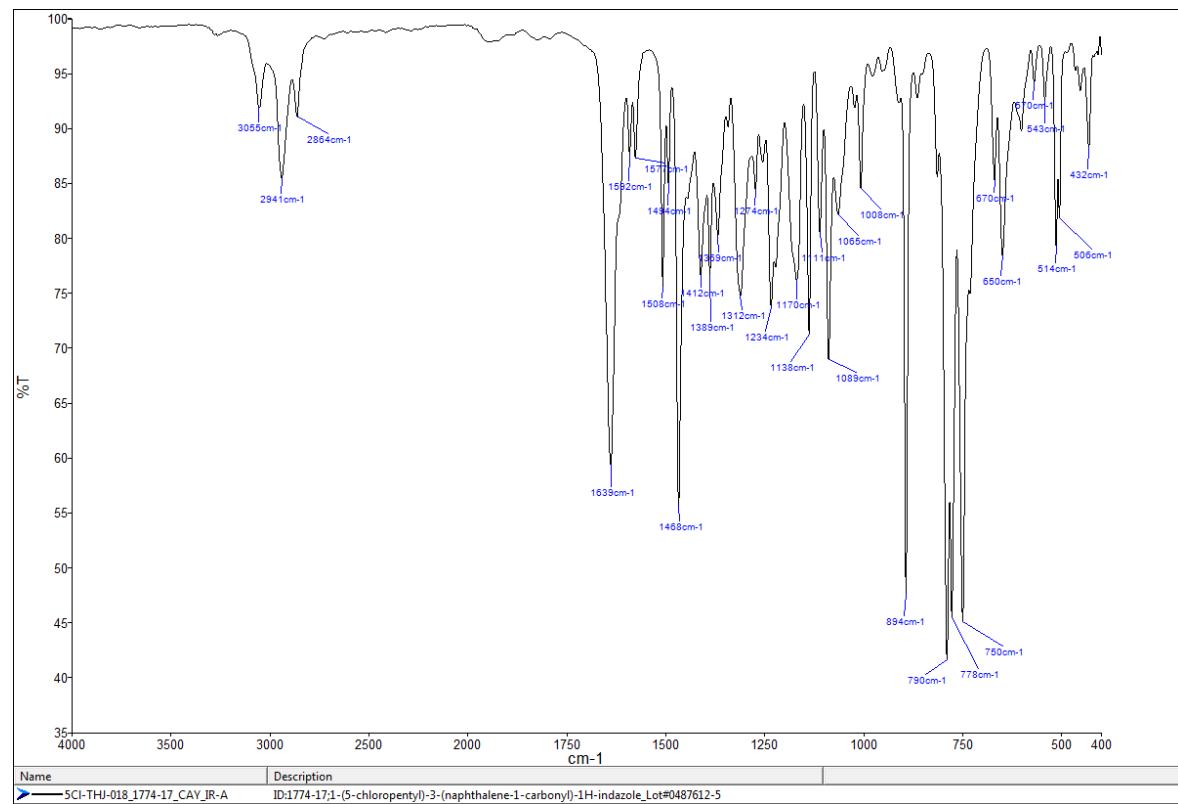

IR (condensed phase – after chromatographic separation)

