



Vodovodna 95
 1000 Ljubljana
 SLOVENIJA

T: +386 (0)1 428 44 93
 E: nfl@policija.si
www.policija.si

ANALYTICAL REPORT

6-MeO-DiPT (C17H26N2O)

[2-(6-methoxy-1H-indol-3-yl)ethyl]bis(propan-2-yl)amine

Remark – other active cpd. detected: **none**

| | |
|-------------------------|--|
| Sample ID: | 1693-16 |
| Sample description: | powder - off white |
| Sample type: | RM-reference material |
| Comments ¹ : | CAY Lot#0474429; I-SEE project RM and report |
| Date of entry: | 10/10/2016 |

| | |
|---|--|
| Substance identified-structure ² (base form) | |
| Systematic name: | [2-(6-methoxy-1H-indol-3-yl)ethyl]bis(propan-2-yl)amine |
| Other names: | 6-methoxy-N,N-Diisopropyltryptamine; 6-Methoxy DiPT; 6-methoxy-N,N-bis(1-methylethyl)-1H-indole-3-ethanamine |
| Formula (per base form) | C17H26N2O |
| M _w (g/mol) | 274,41 |
| Salt form: | HCl |
| StdInChIKey | VVHSFCPALYIWMT-UHFFFAOYSA-N |
| Compound Class | Indolalkylamines (fe tryptamines) |
| Other active cpd. detected | none |
| Add.info (purity..) | 98 % |

¹ This report has been produced with the financial support of the Prevention of and fight against crime Programme of the European Union (grant agreement number JUST/2013/ISEC/DRUGS/AG/6426). The contents of this report are the sole responsibility of the National Forensic Laboratory and can in no way be taken to reflect the views of the European Commission.

² Created by OPSIN free tool: <http://opsin.ch.cam.ac.uk/> DOI: 10.1021/ci100384d

Report updates

| date | comments (explanation) |
|------|------------------------|
| | |
| | |
| | |
| | |

Supporting information

| Analytical technique: | applied | remarks |
|-------------------------|---------|---|
| GC-MS (EI ionization) | + | NFL GC-RT (min): 8.82 BP(1): 114; BP(2): 72, BP(3) :160, |
| FTIR-ATR | + | |
| GC-IR (condensed phase) | + | |

1. GC-MS (Agilent): GC-method is RT locked to tetracosane (9.258 min). Injection volume 1 ml and split mode (1:50). Injector temperature: 280 °C. Chromatographic separation: on column HP1-MS (100% dimethylpolysiloxane), length 30 m, internal diameter 0.25 mm, film thickness 0.25 µm. Carrier gas He: flow-rate 1.2 ml/min. GC oven program: 170 °C for 1 min, followed by heating up to 190 °C at rate 8 °C/min, then heating up to 293 °C at a rate of 18 °C/min, hold for 6.1 min, then heating at 50 °C/min up to 325 °C and finally 6.1 min isothermal. MSD source EI = 70 eV. GC-MS transfer line T= 235 °C, source and quadropole temperatures 280 °C and 180 °C, respectively. Scan range m/z scan range: from 50 (30 until 6 min.) to 550 (300 until 6 min) amu.

2. FTIR-ATR (Perkin Elmer): scan range 4000-400 cm⁻¹; resolution 4cm⁻¹

3. GC- (MS)-IR condensed phase (GC-MS (Agilent) & IR (Spectra analyses-Danny))

GC-method: Injection volume 1 ml and split mode (1:5). Injector temperature 280 °C. Chromatographic separation as above (**1**). Split MS : IR = 1 : 9.


MSD source EI = 70 eV. GC-MS transfer line T= 235 °C, source and quadropole temperatures 280 °C and 180 °C, respectively. Scan range m/z scan range: from 50 (30 until 6 min.) to 550 (300) amu.

IR (condensed solid phase): IR scan range 4000 to 650, resolution 4 cm⁻¹.


FIGURES OF SPECTRA

MS (EI)

Abundance

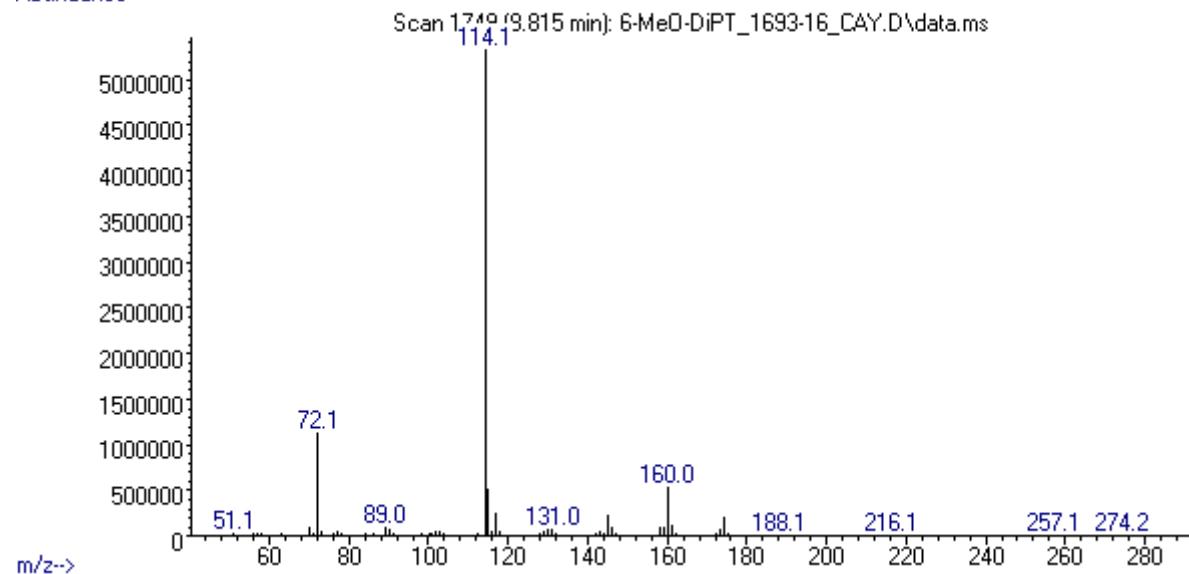

FTIR-ATR (direct measurement)

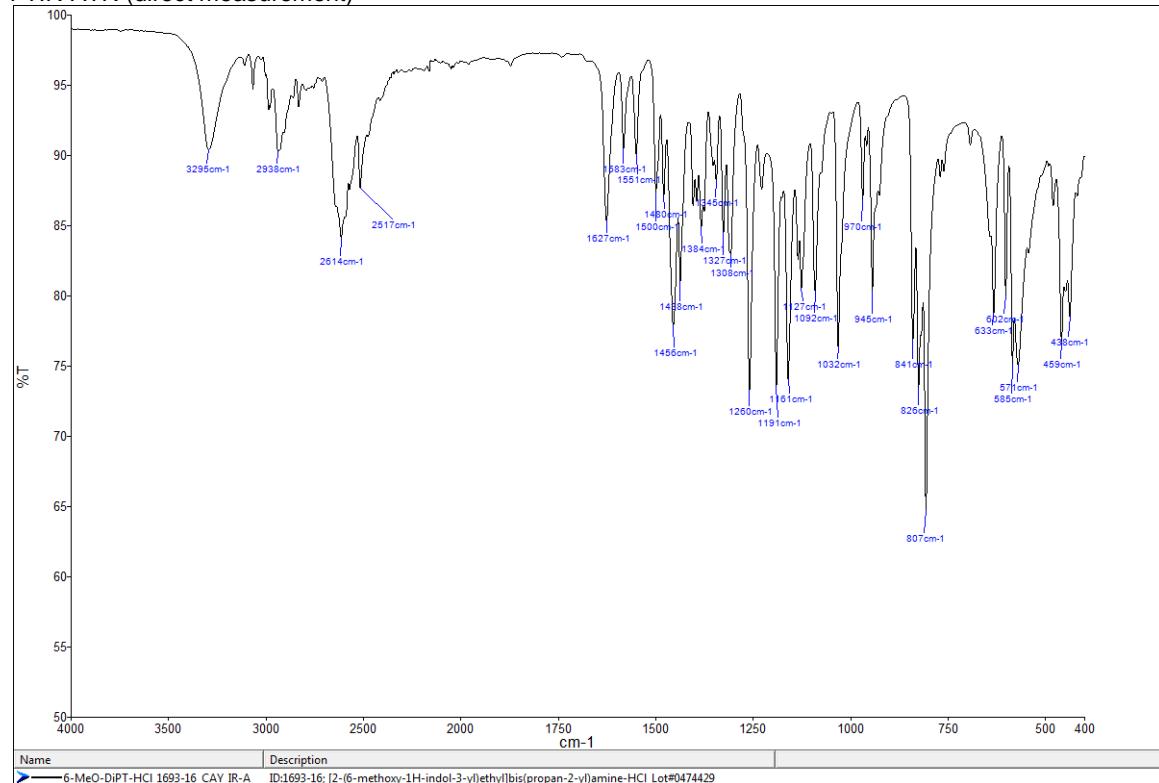

GC-IR-Condensed phase

