NACIONALNI FORENZIČNI LABORATORIJ
NATIONAL FORENSIC LABORATORY
Vodovodna 95, 1000 LJUBLJANA, SLOVENIA
E: nfl@policija.si

EUROPEAN PROJECT RESPONSE 2
to challenges in forensic drugs analyses
S podporo skladov Evropske unije na področju notranjih zadev

ANALYTICAL REPORT

EFLEA (C12H17NO3)

N-[1-(2,3-dihydro-1,4-benzodioxin-6-yl)propan-2-yl]-N-methylhydroxylamine

Remark – other NPS detected:

Sample ID:	1866-17
Sample description:	powder
Sample type:	test purchase /ISF projekt (NFL-SI)
Date of sample receipt (M/D/Y):	10/18/2017
Date of entry (M/D/Y) into NFL database:	1/9/2018
Report updates (if any) will be published here:	http://www.policija.si/apps/nfl_response_web/seznam.php

Substance identified - structure[1] (base form)	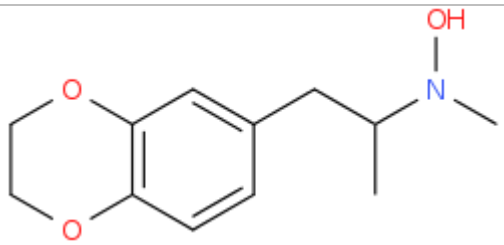
Systematic name	N-[1-(2,3-dihydro-1,4-benzodioxin-6-yl)propan-2-yl]-N-methylhydroxylamine
Other names	N-hydroxy-3,4-ethylenedioxy-N-methylamphetamine; N-Hydroxy-N-methyl-1-(2,3-dihydro-1,4-benzodioxin-6-yl)propane-2-amine; 1-(2,3-Dihydro-1,4-benzodioxin-6-yl)-N-hydroxy-N-methylpropan-2-amine
Formula (per base form)	C12H17NO3
M_w (g/mol)	223,27
Salt form/anions detected	HCl
StdInChIKey (per base form)	FFWSMXIWPUUWNK-UHFFFAOYSA-N
Other NPS detected	
Additional info (purity..)	pure by HPLC-TOF, NMR

[1] Created by OPSIN free tool: http://opsin.ch.cam.ac.uk/ **DOI:** 10.1021/ci100384d

Report updates

date	comments (explanation)

Instrumental methods (if applied) in NFL

1. GC-MS (Agilent): GC-method is RT locked to tetracosane (9.258 min). Injection volume 1 ml and split mode (1:50). Injector temperature: 280 0C. Chromatographic separation: on column HP1-MS (100% dimethylpolysiloxane), length 30 m, internal diameter 0.25 mm, film thickens 0.25 µm. Carrier gas He: flow-rate 1.2 ml/min. GC oven program: 170 ^{0}C for 1 min, followed by heating up to 190 ^{0}C at rate 8 ^{0}C/min, then heating up to 293 0C at a rate of 18 ^{0}C/min, hold for 7.1 min, then heating at 50 ^{0}C/min up to 325 ^{0}C and finally 6.1 min isothermal. MSD source EI = 70 eV. GC-MS transfer line T= 235^{0}C, source and quadropole temperatures 280^{0}C and 180^{0}C, respectively. Scan range m/z scan range: from 50 (30 until 6 min.) to 550 (300 until 6 min) amu.

2. HPLC-TOF (Agilent): 6230B TOF with Agilent 1260 Infinity HPLC with binary pump, column: Zorbax Eclipse XDB-C18, 50 x 4.6 mm, 1.8 micron. Mobile phases (A) 0.1% formic acid and 1mM ammonium formate in water; (B) 0.1% formic acid in methanol (B). Gradient: starting at 5% B, changing to 40% B over 4 min, then to 70% over 2 min and in 5 min to 100%, hold 1 min and back to 5%, equilibration for 1.7 min. The flow rate: 1.0 ml/min; Injection volume 1 µl. MS parameters: 2GHz, Extended Dynamic range mode to a maximum of 1700 amu, acquisition rate 1.30 spectra/sec. Sample ionisation: by Agilent Jet Stream technology (Dual AJS ESI). Ion source: positive ion scan mode with mass scanning from 82 to 1000 amu. Other TOF parameters: drying gas (N2) and sheath temperature 325 °C; drying gas flow rate 6 l/min; sheath gas flow rate 8 l/min; nebulizer 25 psig; Vcap. 4000 V; nozzle 2000 V; skimmer 65 V; fragmentor 175 V and Octopole RF 750 V.

3.FTIR-ATR (Perkin Elmer): scan range 4000-400 cm-1; resolution 4cm-1

4. GC- (MS)-IR condensed phase (GC-MS (Agilent) & IR (Spectra analyses-Danny)
GC-method: Injection volume 1 ml and split mode (1:5). Injector temperature 280 ^{0}C. Chromatographic separation as above **(1).** Split MS : IR = 1: 9.
MSD source EI = 70 eV. GC-MS transfer line T= 235^{0}C, source and quadropole temperatures 280^{0}C and 180^{0}C, respectively. Scan range m/z scan range: from 50 (30 until 6 min.) to 550 (300) amu.
IR (condesed (solid) phase): IR scan range 4000 to 650, resolution 4 cm^{-1}.

5. **IC** (anions) (Thermo Scientific, Dionex ICS 2100), Column: IonPac AS19, 2 x 250mm; Eluent: 10mM from 0 to 10 min, 10-58 mM from 10 to 40min; Flow rate: 0.25 ml/min; Temperature: 30˚C; Suppressor: AERS 500 2mm, suppressor current 13mA; Inj. Volume: 25 µl

Supporting information

Solubility in	result/remark
CH_2Cl_2	partially
MeOH	soluble
H_2O	partially

Analytical technique:	applied	remarks
GC-MS (EI ionization)	+	NFL GC-RT (min): 6,76 (as TMS derivative) BP(1): 146; BP(2): 149,BP(3) :147,
HPLC-TOF	+	Exact mass (theoretical): 223,1208; measured value Δppm:1,07; formula:C12H17NO3
FTIR-ATR	+	direct measurement (sample as received)
FTIR (condensed phase) always as base form	-	
IC (anions)	+	
NMR (in FKKT)	+	
validation		
other		

ANALYTICAL RESULTS

MS (EI) of EFLEA-TMS derivative

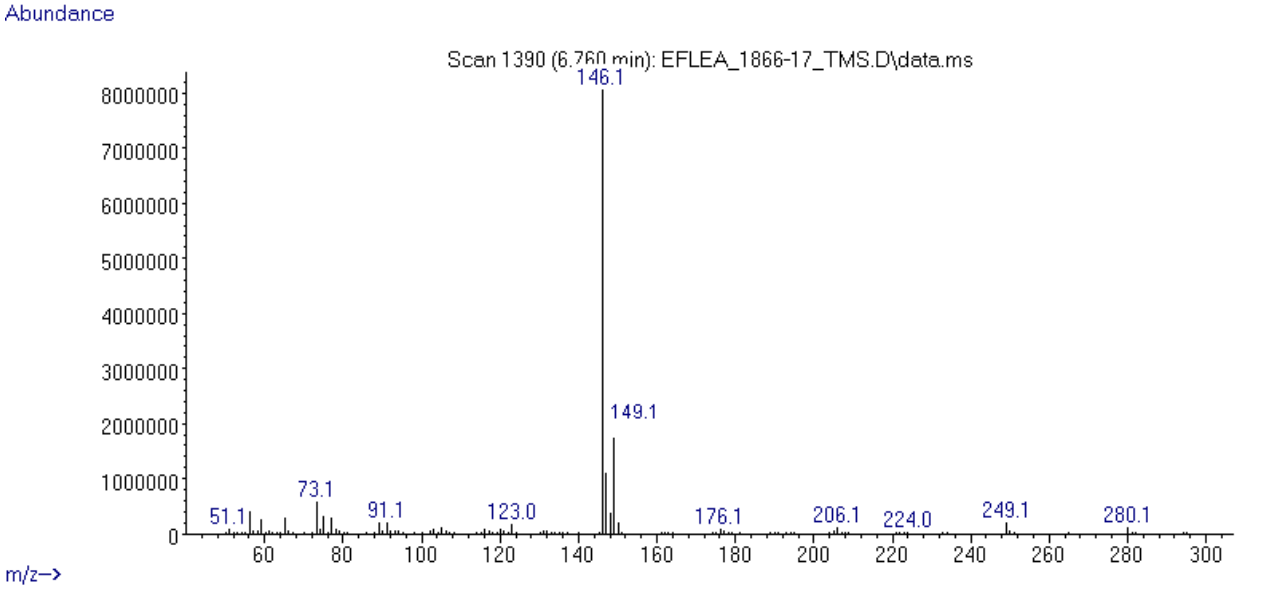

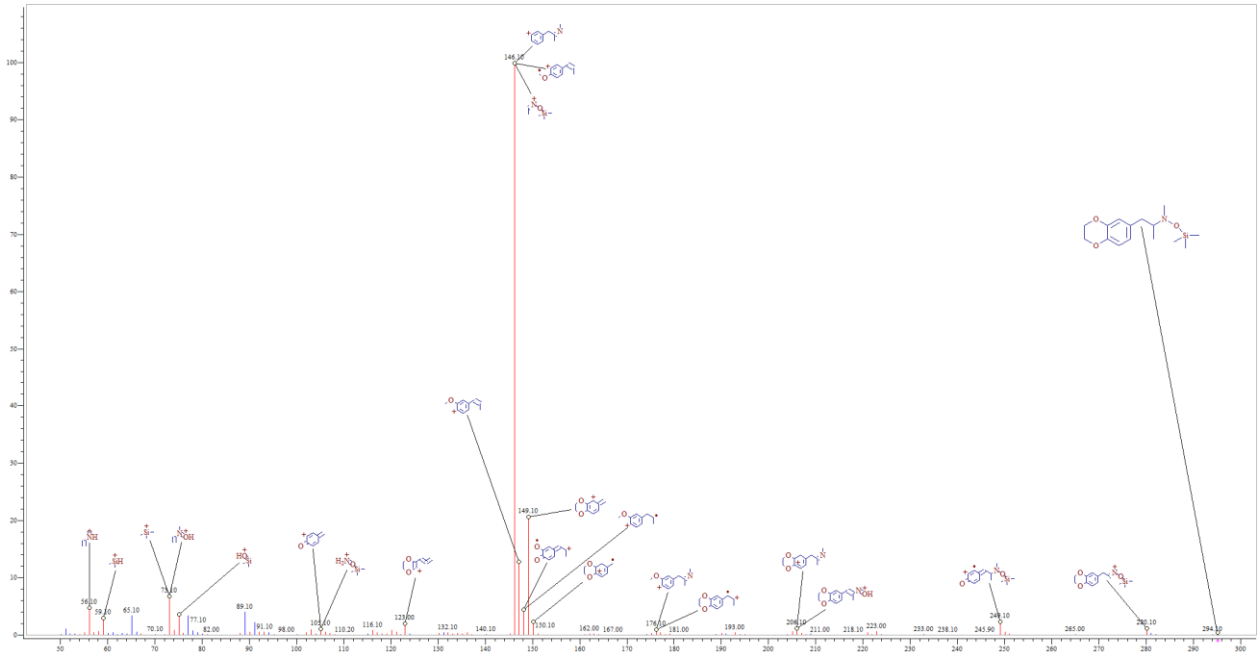

FTIR-ATR - direct measurement (sample as received)

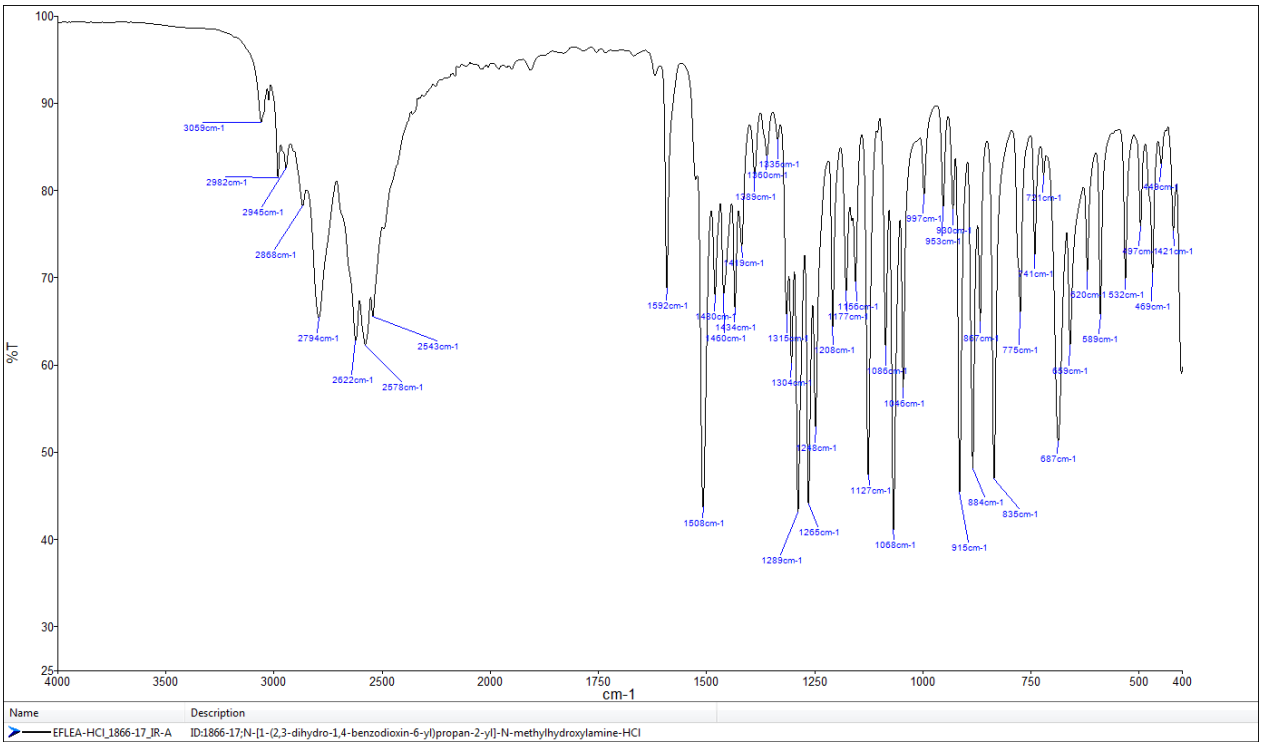

TOF REPORT

Data File	1866-17.d	**Sample Name**	1866-17
Sample Type	Sample	**Position**	P2-A5
Instrument Name	6230B TOF LC-MS	**User Name**	TG
Acq Method	general-19_07_2017-XDB-C18-ESI-final.m	**Acquired Time**	10/20/2017 9:18:13 AM
IRM Calibration Status	Success	**DA Method**	Drugs_NFL.m
Comment	MeOH		

Compound Table

Label	Compound Name	MFG Formula	Obs. RT	Obs. Mass
Cpd 2: EFLEA	EFLEA	C12 H17 N O3	5.18	223.1206

Name	*Obs. m/z*	Obs. RT	Obs. Mass	DB RT	DB Formula	DB Mass	DB Mass Error (ppm)
EFLEA	224.1281	5.18	223.1206	5.18	C12 H17 N O3	223.1208	1.07

Compound Chromatograms

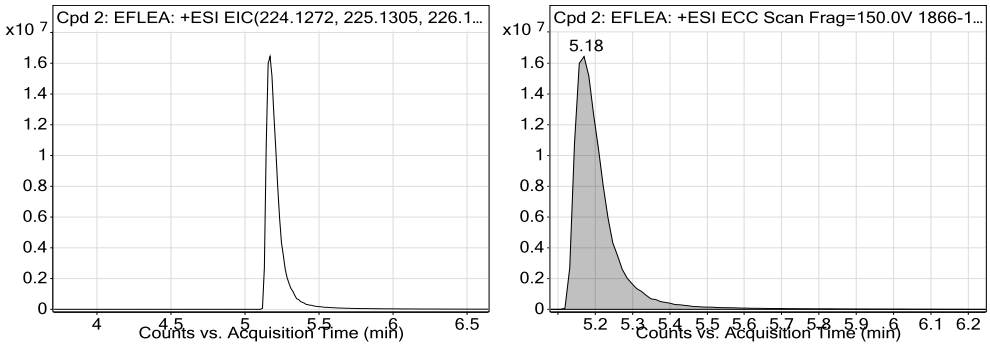

MFE MS Zoomed Spectrum

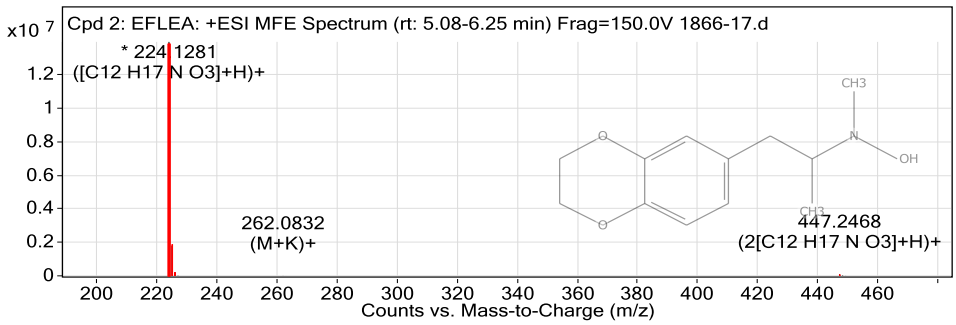

MS Zoomed Spectrum

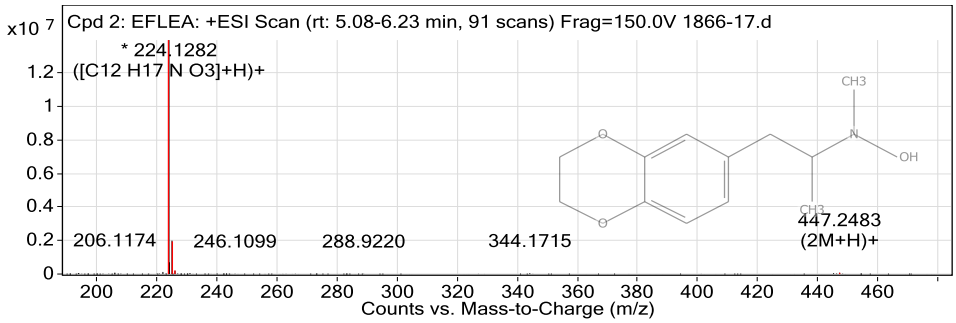

MS Spectrum Peak List

Obs. m/z	Charge	Abund	Formula	Ion/Isotope
224.1281	1	13944696	C12 H17 N O3	(M+H)+
225.1298	1	1776243.09	C12 H17 N O3	(M+H)+
226.1321	1	179255.35	C12 H17 N O3	(M+H)+
227.1346	1	15704.16	C12 H17 N O3	(M+H)+
262.0832	1	4273.74		(M+K)+
263.0771	1	1348.45		(M+K)+
447.2468	1	102871.11	C12 H17 N O3	(2M+H)+
448.2503	1	26225.25	C12 H17 N O3	(2M+H)+
449.2529	1	4849.88	C12 H17 N O3	(2M+H)+

--- End Of Report ---

Peak Integration Report

Sample Name:	**1866-17**	*Inj. Vol.:*	**25,00**
Injection Type:	**Unknown**	*Dilution Factor:*	**1,0000**
Program:	**ANIONI**	*Operator:*	**kemija**
Inj. Date / Time:	**20-okt-2017 / 11:25**	*Run Time:*	**42,00**

No.	Time min	Peak Name	Peak Type	Area µS*min	Height µS	Amount mg/L
1,00	9,35	**Chloride**	BMB	3,17	14,72	n.a.
		TOTAL:		3,17	14,72	0,00

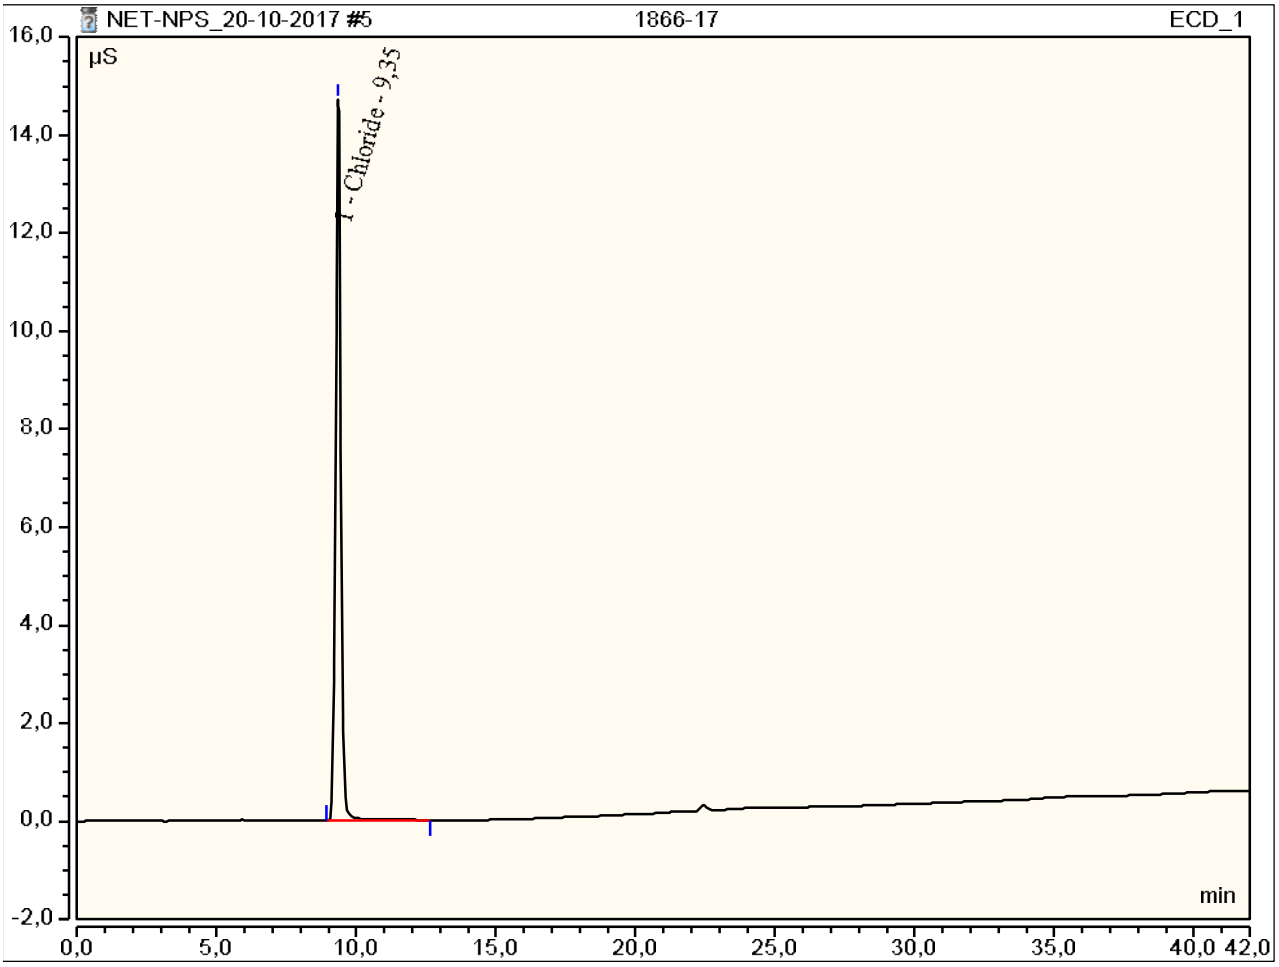

Večna pot 113
P. O. Box 537
SI-1001 Ljubljana
Slovenia
Phone: +386 1 479 8558
janez.kosmrlj@fkkt.uni-lj.si

University
of Ljubljana

Faculty *of Chemistry*
and Chemical Technology

R E P O R T

Contract No.	C1714-17-460078 (Republic of Slovenia, Ministry of the Interior, POLICE)
Sample ID:	**1866-17**
Received date:	December 8, 2017
Our notebook code:	NFL-1866-17
NMR sample preparation:	16.5 mg dissolved in 0.7 mL DMSO-d_6
NMR experiments:	^{1}H, ^{13}C, ^{1}H–^{1}H *gs*-COSY, ^{1}H–^{13}C *gs*-HSQC, ^{1}H–^{13}C *gs*-HMBC, ^{1}H–^{15}N *gs*-HMBC
Proposed structure, formula, exact mass, molecular weight:	 Chemical Formula: $C_{12}H_{18}NO_3^+$ Exact Mass: 224,1281 Molecular Weight: 224,2795
Chemical name:	N-protonated *N*-(1-(2,3-dihydrobenzo[b][1,4]dioxin-6-yl)propan-2-yl)-*N*-methylhydroxylamine
Comments:	- Structure elucidation based on 1D and 2D NMR spectra and HRMS. - >98% purity of the sample based on ^{1}H NMR spectrum
Supporting information:	Copies of ^{1}H and ^{13}C NMR spectra, ^{1}H and ^{13}C FIDs
Principal investigator:	Prof. Dr. Janez Košmrlj
Date of report:	December 22, 2017

NFL-1866-17
1H

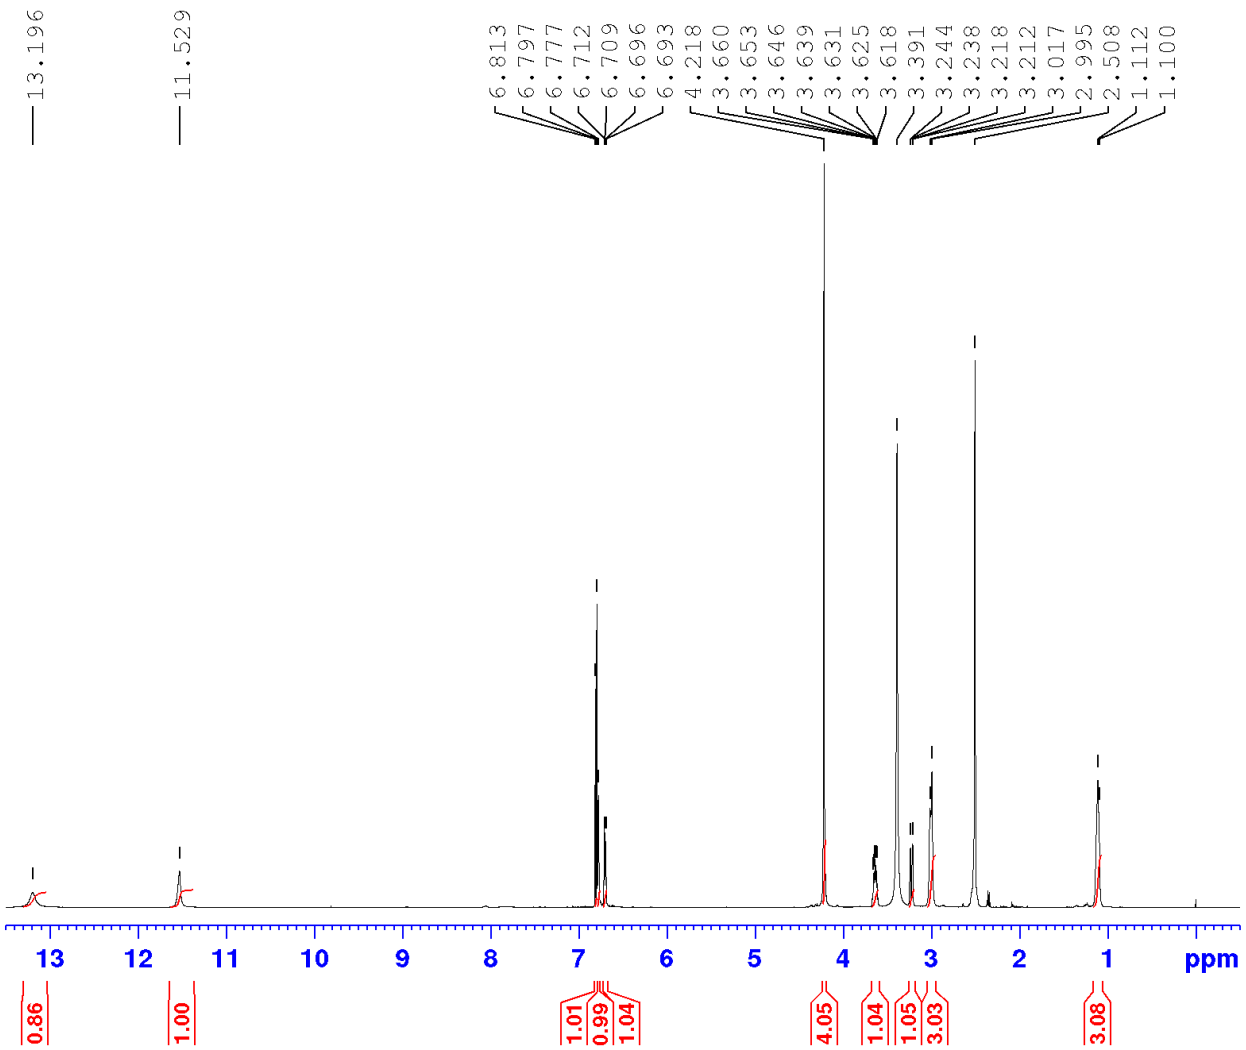


```
Current Data Parameters
NAME         NFL-1866-17
EXPNO                  2
PROCNO                 1

F2 - Acquisition Parameters
Date_           20171211
Time               17.55
INSTRUM            spect
PROBHD   5 mm PABBO BB-
PULPROG             zg30
TD                 65536
SOLVENT             DMSO
NS                    16
DS                     2
SWH            10000.000 Hz
FIDRES          0.152588 Hz
AQ             3.2767999 sec
RG                  80.6
DW                50.000 usec
DE                 6.50 usec
TE                296.0 K
D1            1.00000000 sec
TD0                    1

======== CHANNEL f1 ========
SFO1         500.1330885 MHz
NUC1                   1H
P1                  8.70 usec
PLW1         26.00000000 W

F2 - Processing parameters
SI                 65536
SF           500.1300005 MHz
WDW                   EM
SSB       0
LB                 0.30 Hz
GB        0
PC                 1.00
```

NFL-1866-17
13C

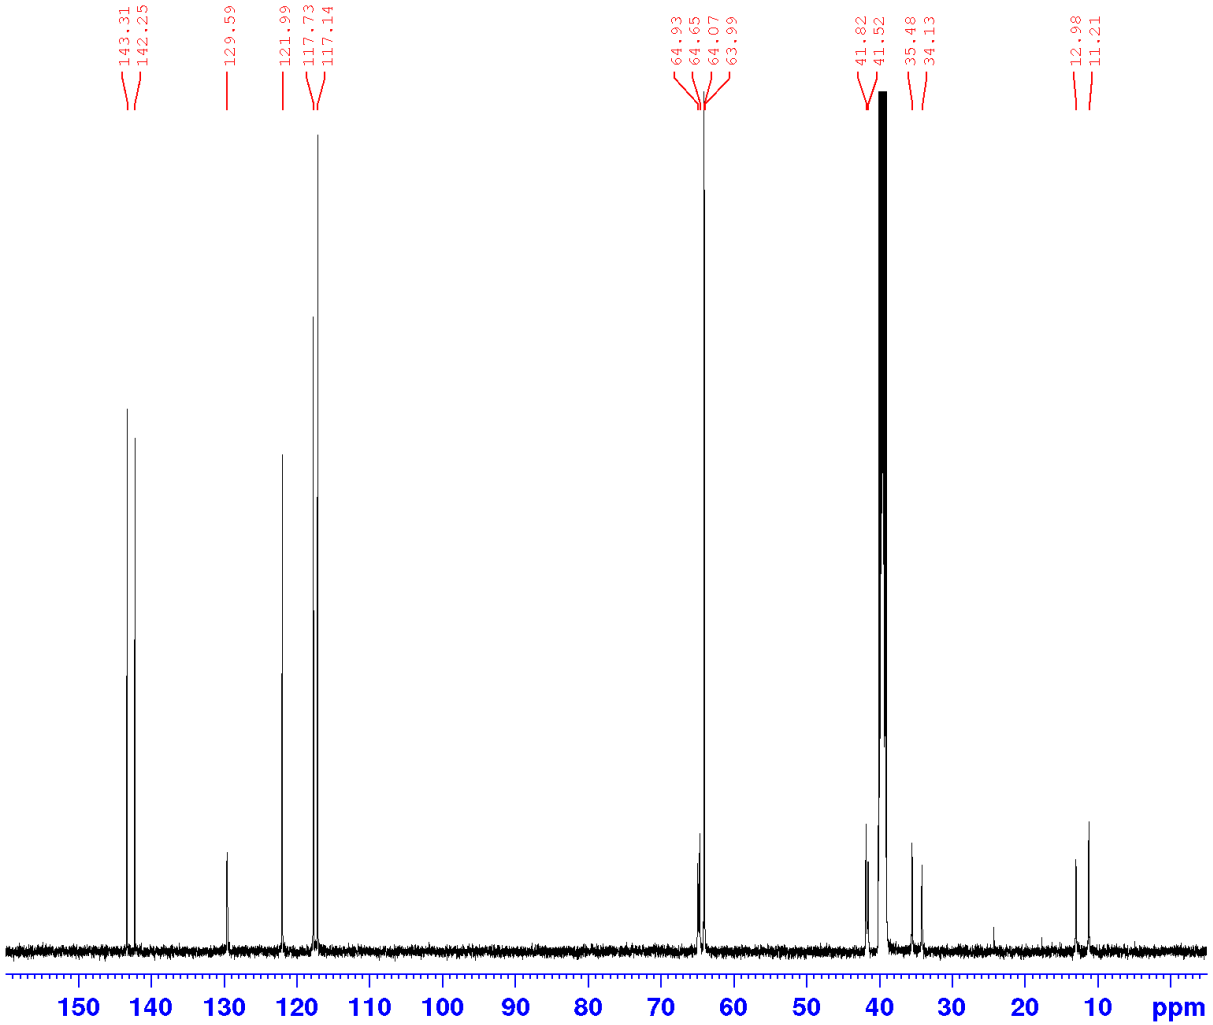


```
Current Data Parameters
NAME         NFL-1866-17
EXPNO                  8
PROCNO                 1

F2 - Acquisition Parameters
Date_           20171215
Time                7.31
INSTRUM            spect
PROBHD   5 mm PABBO BB-
PULPROG          zgpg30
TD                65536
SOLVENT             DMSO
NS                  5120
DS                     4
SWH           29761.904 Hz
FIDRES         0.454131 Hz
AQ             1.1010048 sec
RG                  2050
DW               16.800 usec
DE                6.50 usec
TE                296.0 K
D1           2.00000000 sec
D11          0.03000000 sec
TD0                    1

======== CHANNEL f1 ========
SFO1        125.7703637 MHz
NUC1                  13C
P1                 8.70 usec
PLW1       122.00000000 W

======== CHANNEL f2 ========
SFO2        500.1320005 MHz
NUC2                  1H
CPDPRG[2         waltz16
PCPD2             80.00 usec
PLW2         26.00000000 W
PLW12         0.30046001 W
PLW13         0.15113001 W

F2 - Processing parameters
SI                 32768
SF          125.7578438 MHz
WDW                   EM
SSB       0
LB                 1.00 Hz
GB        0
PC                 1.40
```