NACIONALNI FORENZIČNI LABORATORIJ
NATIONAL FORENSIC LABORATORY

Vodovodna 95
1000 Ljubljana
SLOVENIJA

T: +386 (0)1 428 44 93
E: nfl@policija.si
www.policija.si

ANALYTICAL REPORT[1]

FUB-PB22 (C25H17FN2O2)

1-[(4-fluorophenyl)methyl]-1H-indole-3-carboxylic acid, 8-quinolinyl ester

Remark – other NPS detected: none

Sample ID:	1286-15
Sample description:	powder - white
Sample type:	test purchase /RESPONSE -purchasing
Date of sample receipt (M/D/Y):	8/18/2015
Date of entry (M/D/Y) into NFL database:	10/4/2015
Report updates (if any) will be published here:	http://www.policija.si/apps/nfl_response_web/seznam.php

Substance identified - structure[2] (base form)	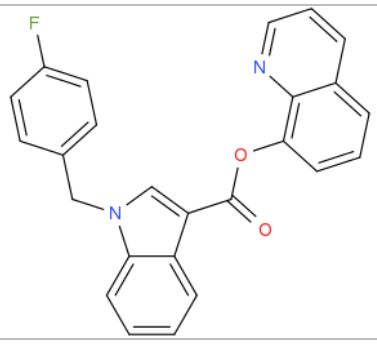
Systematic name	1-[(4-fluorophenyl)methyl]-1H-indole-3-carboxylic acid, 8-quinolinyl ester
Other names	
Formula (per base form)	C25H17FN2O2
M_w (g/mol)	396,41
Salt form	
StdInChIKey	ROHVURVXAOMRJY-UHFFFAOYSA-N
Compound Class	Cannabinoids
Other NPS detected	none
Add.info (purity..)	pure by GC-MS, HPLC-TOF

[1] This report has been produced with the financial support of the Prevention of and fight against crime Programme of the European Union (grant agreement number JUST/2013/ISEC/DRUGS/AG/6413). The contents of this report are the sole responsibility of the National Forensic Laboratory and can in no way be taken to reflect the views of the European Commission.

[2] Created by OPSIN free tool: http://opsin.ch.cam.ac.uk/ **DOI:** 10.1021/ci100384d

Report updates

date	comments (explanation)

Instrumental methods (if applied) in NFL

1. GC-MS (Agilent): GC-method is RT locked to tetracosane (RT=9.53 min). Injection volume 1 ml and split mode (1:50) . Injector temperature: 280 ^{0}C. Chromatographic separation: on column HP1-MS (100% dimethylpolysiloxane), length 30 m, internal diameter 0.25 mm, film thickens 0.25 mm. Carrier gas He: flow-rate 1.2 ml/min. GC oven program: 170 ^{0}C for 1 min, followed by heating up to 293 ^{0}C at a rate of 18 ^{0}C/min, hold for 6.1 min, than heating at 50 ^{0}C/min up to 325 ^{0}C and finally 2.8 min isothermal. MSD source EI = 70 eV. GC-MS transfer line T= 235^{0}C, source and quadropole temperatures 280^{0}C and 180^{0}C, respectively. Scan range m/z scan range: from 50 (40) to 550 amu.

2. HPLC-TOF (Agilent): 6230B TOF with Agilent 1260 Infinity HPLC with binary pump, column: Zorbax Eclipse XDB-C18, 50 x 4.6 mm, 1.8 micron. Mobile phases (A) 0.1% formic acid and 1mM ammonium formate in water; (B) 0.1% formic acid in methanol (B). Gradient: starting at 5% B, changing to 40% B over 4 min, then to 70% over 2 min and in 5 min to 100%, hold 1 min and back to 5%, equilibration for 1.7 min. The flow rate: 1.0 ml/min; Injection volume 1 µl. MS parameters: 2GHz, Extended Dynamic range mode to a maximum of 1700 amu, acquisition rate 1.30 spectra/sec. Sample ionisation: by Agilent Jet Stream technology (Dual AJS ESI). Ion source: positive ion scan mode with mass scanning from 82 to 1000 amu. Other TOF parameters: drying gas (N2) and sheath temperature 325 °C; drying gas flow rate 6 l/min; sheath gas flow rate 8 l/min; nebulizer 25 psig; Vcap. 4000 V; nozzle 2000 V; skimmer 65 V; fragmentor 175 V and Octopole RF 750 V.

3.FTIR-ATR (Perkin Elmer): scan range 4000-400 cm-1; resolution 4cm-1

4. GC- (MS)-IR condensed phase (GC-MS (Agilent) & IR (Spectra analyses-Danny)
GC-method: Injection volume 1 ml and split mode (1:5). Injector temperature 280 ^{0}C. Chromatographic separation as above **(1).**
Split MS : IR = 1:9.
MSD source EI = 70 eV. GC-MS transfer line T= 235^{0}C, source and quadropole temperatures 280^{0}C and 180^{0}C, respectively. Scan range m/z scan range: from 50 (40) to 550 amu.
IR (condesed phase): IR scan range 4000 to 650, resolution 4 cm^{-1}.

5. **IC** (anions) (Thermo Scientific, Dionex ICS 2100), Column: IonPac AS19, 2 x 250mm; Eluent: 10mM from 0 to 10 min, 10-58 mM from 10 to 40min; Flow rate: 0.25 ml/min; Temperature: 30˚C; Suppressor: AERS 500 2mm, suppressor current 13mA; Inj. Volume: 25 µl

Supporting information

Solubility in	result/remark
CH_2Cl_2	partially
MeOH	soluble
H_2O	

Analytical technique:	applied	remarks
GC-MS (EI ionization)	+	NFL GC-RT (min): 18,92 BP(1): 109; BP(2): 252,BP(3) :253,
HPLC-TOF	+	Exact mass (theoretical): 396,1274; measured value Δppm:0,43; formula:C25H17FN2O2
FTIR-ATR	+	direct measurement (sample as received)
FTIR (condensed phase) always as base form	+	
IC (anions)	+	
NMR (in FKKT)	-	
validation		FTIR-ATR consistent with the one from SWGDRUG IR library http://www.swgdrug.org/ir.htm ; (QM<0.996), entry LOT RM-131008-01
other		

ANALYTICAL RESULTS

MS (EI)

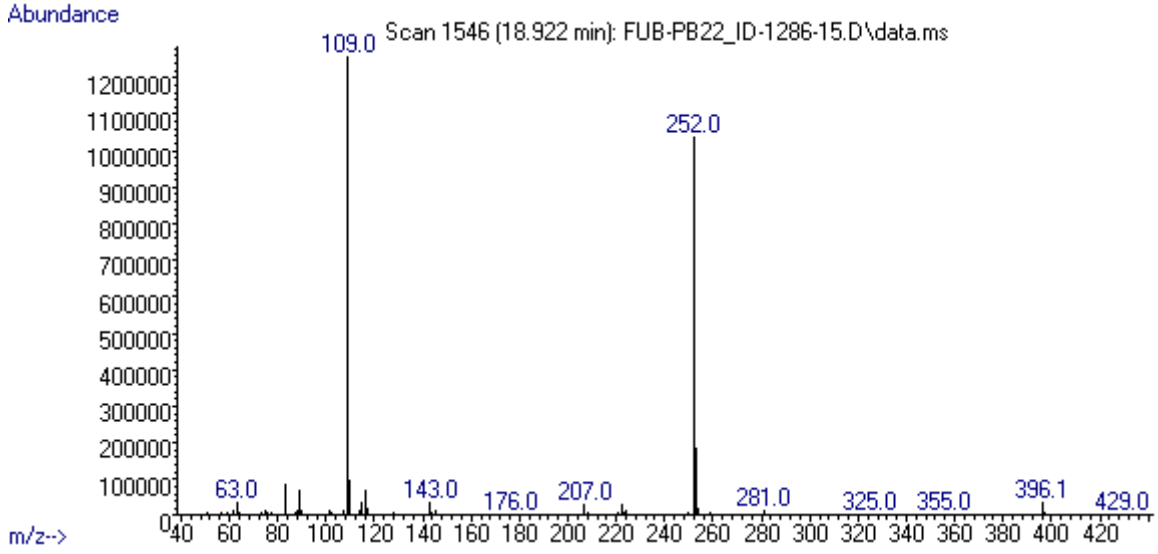

FTIR-ATR - direct measurement (sample as received)

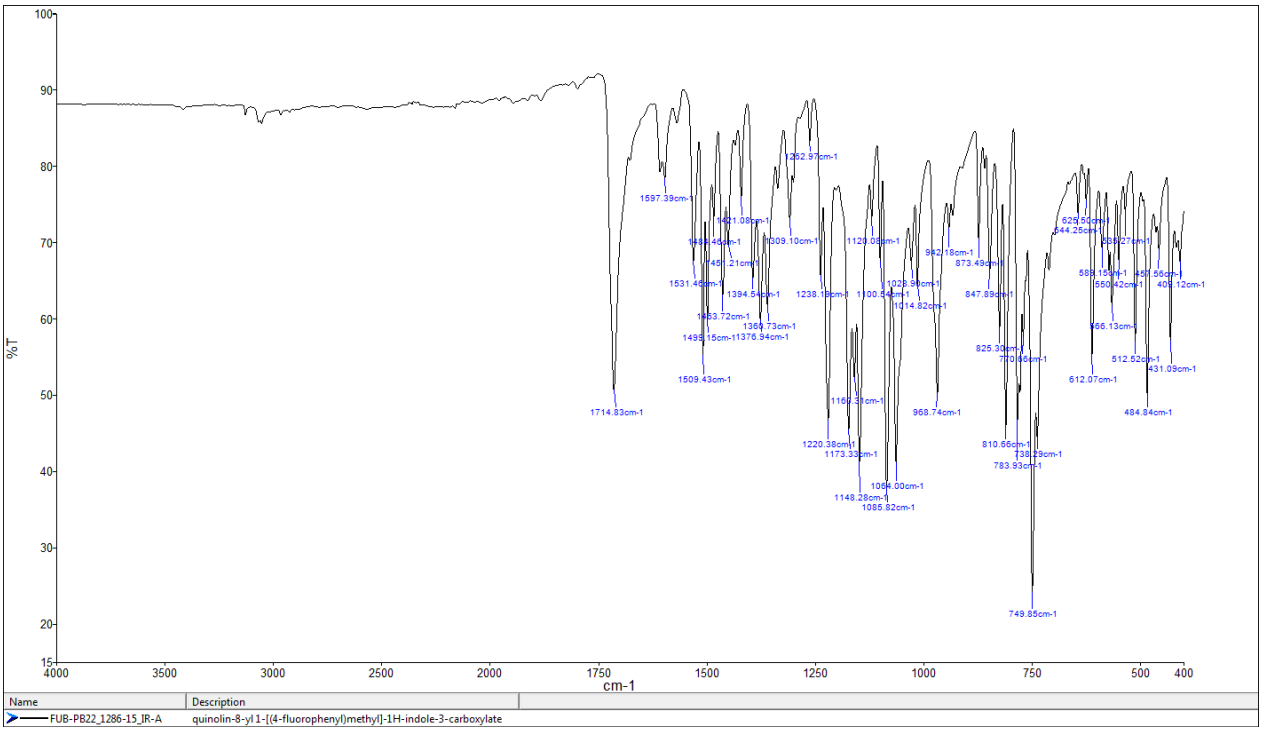

IR (condensed phase – after chromatographic separation)

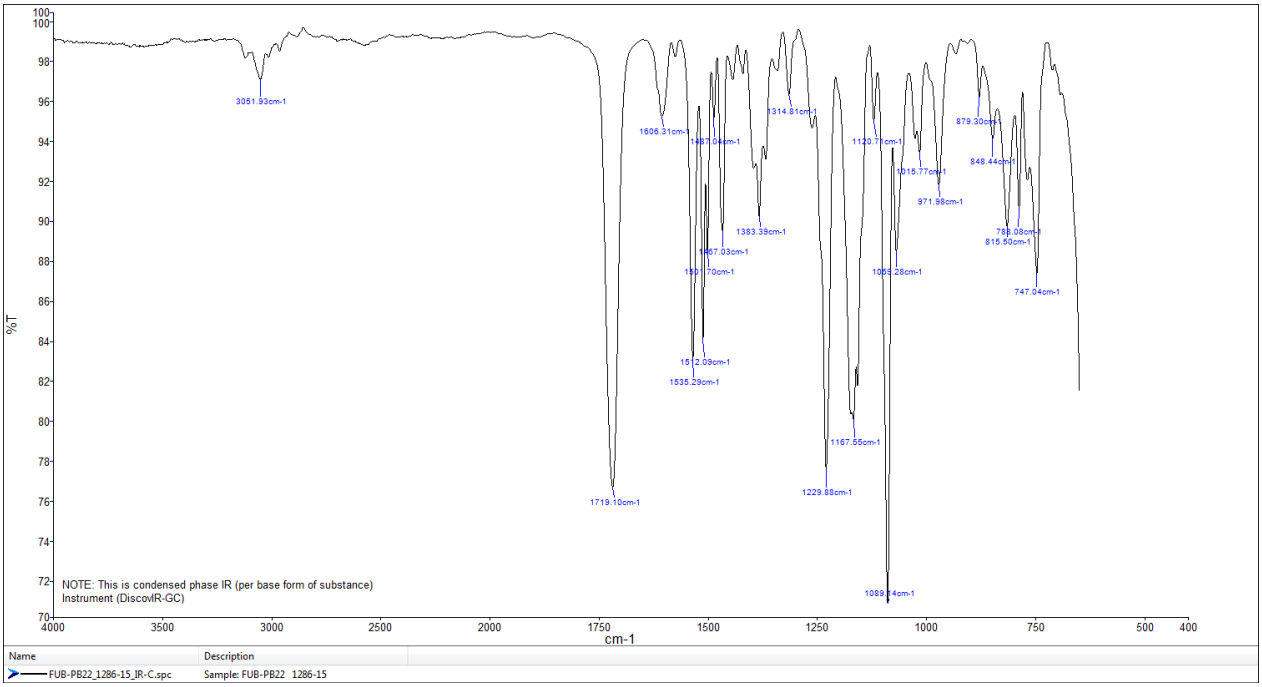

ID 1286-15

TOF REPORT

Data File	FUB-PB22_1286-15_TOF.d	**Sample Name**	FDU-PB22
Sample Type	Sample	**Position**	P1-F2
Instrument Name	6230B TOF LC-MS	**User Name**	TG
Acq Method	droge general-13-5-2015-XDB-C18-ESI-poz.m	**Acquired Time**	9/21/2015 9:28:54 AM
IRM Calibration Status	Success	**DA Method**	Drugs_NFL.m
Comment	extract in MeOH		

Compound Table

Label	Compound Name	Obs. RT	Obs. Mass
Cpd 1: FUB-PB22	FUB-PB22	9.086	396.1272

Name	*Obs. m/z*	Obs. RT	Obs. Mass	DB RT	DB Formula	DB Mass	DB Mass Error (ppm)
FUB-PB22	793.2618	9.086	396.1272	9.127	C25 H17 F N2 O2	396.1274	0.43

Compound Chromatograms

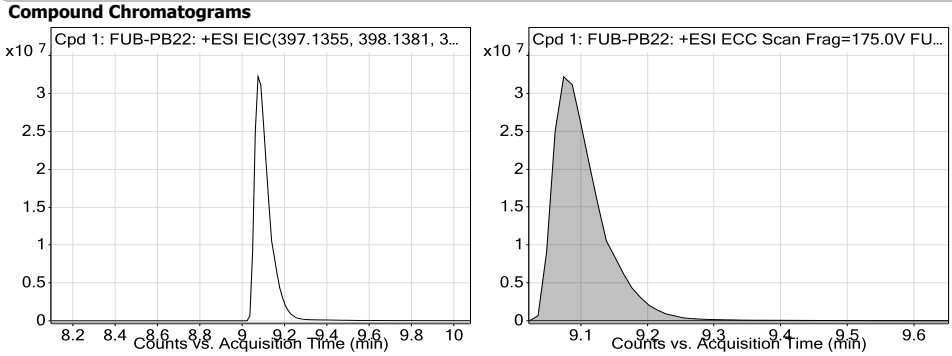

MFE MS Zoomed Spectrum

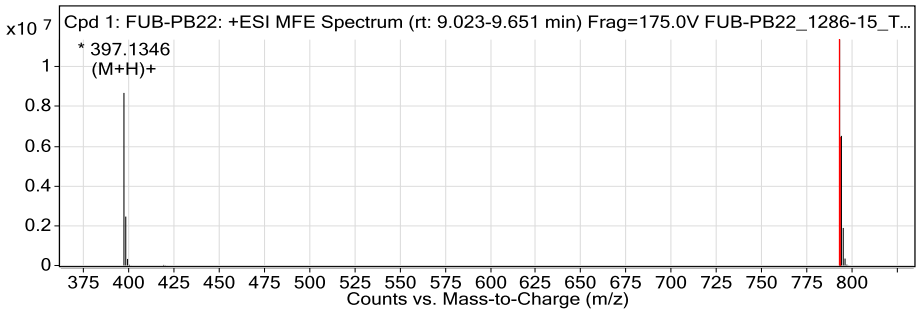

MS Zoomed Spectrum

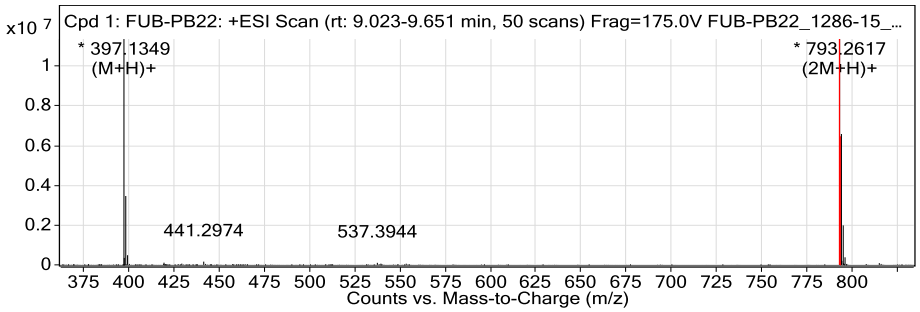

MS Spectrum Peak List

Obs. m/z	Charge	Abund	Formula	Ion/Isotope
397.1346	1	8685879		(M+H)+
398.1382	1	2460400.44		(M+H)+
399.1415	1	328774.82		(M+H)+
400.1439	1	32965.88		(M+H)+
419.1164	1	28656.25		(M+Na)+
793.2618	1	11366278	C25 H17 F N2 O2	(2M+H)+
794.2652	1	6523153.68	C25 H17 F N2 O2	(2M+H)+
795.2685	1	1889406.79	C25 H17 F N2 O2	(2M+H)+
796.2721	1	347363.59	C25 H17 F N2 O2	(2M+H)+
797.2743	1	42918.79	C25 H17 F N2 O2	(2M+H)+

--- End Of Report ---

Peak Integration Report

Sample Name:	**FUB-PB22_1286-15_IC**	*Inj. Vol.:*	**25,00**
Injection Type:	**Unknown**	*Dilution Factor:*	**1,0000**
Program:	**ANIONI**	*Operator:*	**kemija**
Inj. Date / Time:	**27-okt-2015 / 19:43**	*Run Time:*	**42,00**

No.	Time min	Peak Name	Peak Type	Area µS*min	Height µS	Amount n.a.
		TOTAL:		0,00	0,00	0,00