




## ANALYTICAL REPORT<sup>1</sup>

### MDAI (C<sub>10</sub>H<sub>11</sub>NO<sub>2</sub>)

#### 2H,5H,6H,7H-indeno[5,6-d][1,3]dioxol-6-amine

Remark – other NPS detected: **none**

Sample ID:	1347-15
Sample description:	crystallinic - off white
Sample type:	test purchase /RESPONSE -purchasing
Date of sample receipt (M/D/Y):	11/6/2015
Date of entry (M/D/Y) into NFL database:	11/25/2015
Report updates (if any) will be published here:	<a href="http://www.policija.si/apps/nfl_response_web/seznam.php">http://www.policija.si/apps/nfl_response_web/seznam.php</a>

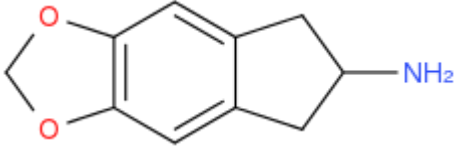Substance identified - structure <sup>2</sup> (base form)	
Systematic name	2H,5H,6H,7H-indeno[5,6-d][1,3]dioxol-6-amine
Other names	5,6-methylenedioxy-2-aminoindane
Formula (per base form)	C <sub>10</sub> H <sub>11</sub> NO <sub>2</sub>
M <sub>w</sub> (g/mol)	177,2
Salt form	HCl
StdInChIKey	FQDRMHHCWZAXJM-UHFFFAOYSA-N
Compound Class	Aminoindanes
Other NPS detected	none
Add.info (purity..)	

<sup>1</sup> This report has been produced with the financial support of the Prevention of and fight against crime Programme of the European Union (grant agreement number JUST/2013/ISEC/DRUGS/AG/6413). The contents of this report are the sole responsibility of the National Forensic Laboratory and can in no way be taken to reflect the views of the European Commission.

<sup>2</sup> Created by OPSIN free tool: <http://opsin.ch.cam.ac.uk/> DOI: 10.1021/ci100384d

## Report updates

date	comments (explanation)

### Instrumental methods (if applied) in NFL

**1. GC-MS** (Agilent): GC-method is RT locked to tetracosane (RT=9.53 min). Injection volume 1 ml and split mode (1:50) . Injector temperature: 280 °C. Chromatographic separation: on column HP1-MS (100% dimethylpolysiloxane), length 30 m, internal diameter 0.25 mm, film thickness 0.25 mm. Carrier gas He: flow-rate 1.2 ml/min. GC oven program: 170 °C for 1 min, followed by heating up to 293 °C at a rate of 18 °C/min, hold for 6.1 min, then heating at 50 °C/min up to 325 °C and finally 2.8 min isothermal. MSD source EI = 70 eV. GC-MS transfer line T= 235°C, source and quadropole temperatures 280°C and 180°C, respectively. Scan range m/z scan range: from 50 (40) to 550 amu.

**2. HPLC-TOF** (Agilent): 6230B TOF with Agilent 1260 Infinity HPLC with binary pump, column: Zorbax Eclipse XDB-C18, 50 x 4.6 mm, 1.8 micron. Mobile phases (A) 0.1% formic acid and 1mM ammonium formate in water; (B) 0.1% formic acid in methanol (B). Gradient: starting at 5% B, changing to 40% B over 4 min, then to 70% over 2 min and in 5 min to 100%, hold 1 min and back to 5%, equilibration for 1.7 min. The flow rate: 1.0 ml/min; Injection volume 1 µl. MS parameters: 2GHz, Extended Dynamic range mode to a maximum of 1700 amu, acquisition rate 1.30 spectra/sec. Sample ionisation: by Agilent Jet Stream technology (Dual AJS ESI). Ion source: positive ion scan mode with mass scanning from 82 to 1000 amu. Other TOF parameters: drying gas (N<sub>2</sub>) and sheath temperature 325 °C; drying gas flow rate 6 l/min; sheath gas flow rate 8 l/min; nebulizer 25 psig; Vcap. 4000 V; nozzle 2000 V; skimmer 65 V; fragmentor 175 V and Octopole RF 750 V.

**3. FTIR-ATR** (Perkin Elmer): scan range 4000-400 cm<sup>-1</sup>; resolution 4cm<sup>-1</sup>

**4. GC- (MS)-IR** condensed phase (GC-MS (Agilent) & IR (Spectra analyses-Danny)

GC-method: Injection volume 1 ml and split mode (1:5). Injector temperature 280 °C. Chromatographic separation as above **(1)**. Split MS : IR = 1:9.

MSD source EI = 70 eV. GC-MS transfer line T= 235°C, source and quadropole temperatures 280°C and 180°C, respectively. Scan range m/z scan range: from 50 (40) to 550 amu.

IR (condensed phase): IR scan range 4000 to 650, resolution 4 cm<sup>-1</sup>.

**5. IC** (anions) (Thermo Scientific, Dionex ICS 2100), Column: IonPac AS19, 2 x 250mm; Eluent: 10mM from 0 to 10 min, 10-58 mM from 10 to 40min; Flow rate: 0.25 ml/min; Temperature: 30°C; Suppressor: AERS 500 2mm, suppressor current 13mA; Inj. Volume: 25 µl

## Supporting information


Solubility in	result/remark
CH <sub>2</sub> Cl <sub>2</sub>	partially
MeOH	soluble
H <sub>2</sub> O	

Analytical technique:	applied	remarks
GC-MS (EI ionization)	+	NFL GC-RT (min): 4,31 BP(1): 160; BP(2): 149,BP(3) :177,
HPLC-TOF	+	Exact mass (theoretical): 177,079; measured value Δppm:-1,14; formula:C10H11NO2
FTIR-ATR	+	direct measurement (sample as received)
FTIR (condensed phase) always as base form		
IC (anions)	+	
NMR (in FKKT)	-	
validation		MS consistentSWGDRUG.L (QM 0.99), IR fit with Forensic drugs FD044 (entry)
other		


# ANALYTICAL RESULTS

MS (EI)

Abundance

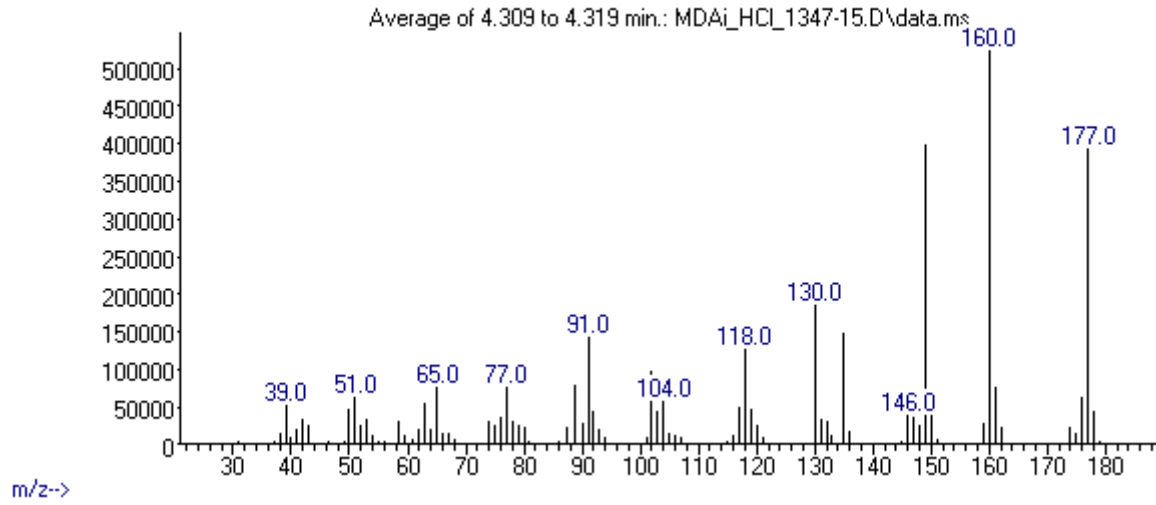

## FTIR-ATR - direct measurement (sample as received)

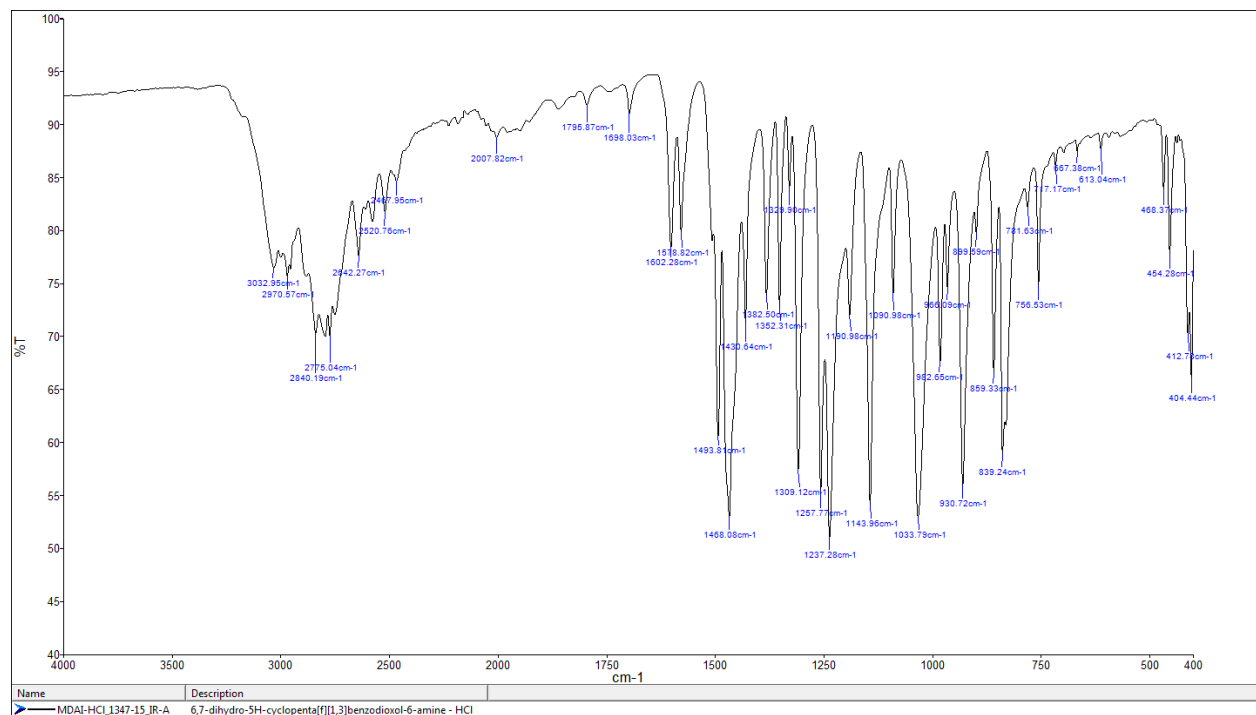

## IR (condensed phase – after chromatographic separation)

# TOF REPORT


<b>Data File</b>	MDAi-1347-15_TOF.d	<b>Sample Name</b>	ID_1347-15
<b>Sample Type</b>	Sample	<b>Position</b>	P1-A2
<b>Instrument Name</b>	6230B TOF LC-MS	<b>User Name</b>	TG
<b>Acq Method</b>	general-17112015-XDB-C18-ESI-poz.m	<b>Acquired Time</b>	11/17/2015 9:30:27 AM
<b>IRM Calibration Status</b>	Success	<b>DA Method</b>	Drugs_NFL.m
<b>Comment</b>	extract in MeOH		

## Compound Table


Label	Compound Name	Obs. RT	Obs. Mass
Cpd 3: MDAI	MDAI	3.367	177.0792

Name	Obs. m/z	Obs. RT	Obs. Mass	DB RT	DB Formula	DB Mass	DB Mass Error (ppm)
MDAI	178.0864	3.367	177.0792	3.4	C10 H11 N O2	177.079	-1.14


## Compound Chromatograms

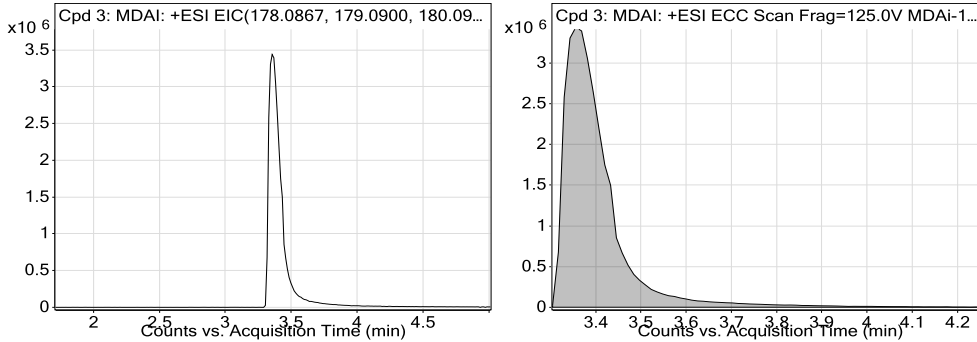

## MFE MS Zoomed Spectrum

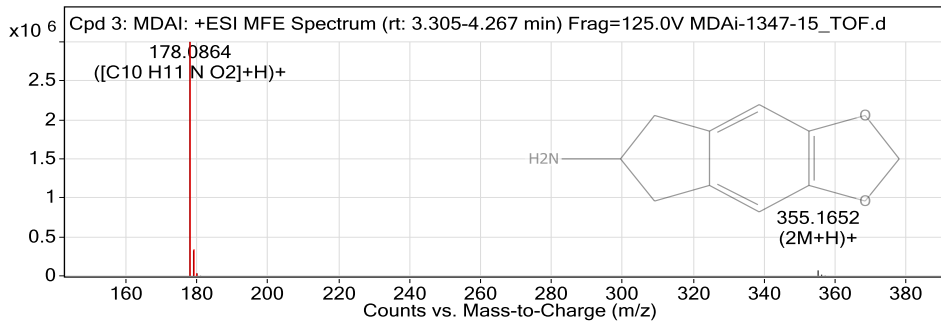

## MS Zoomed Spectrum

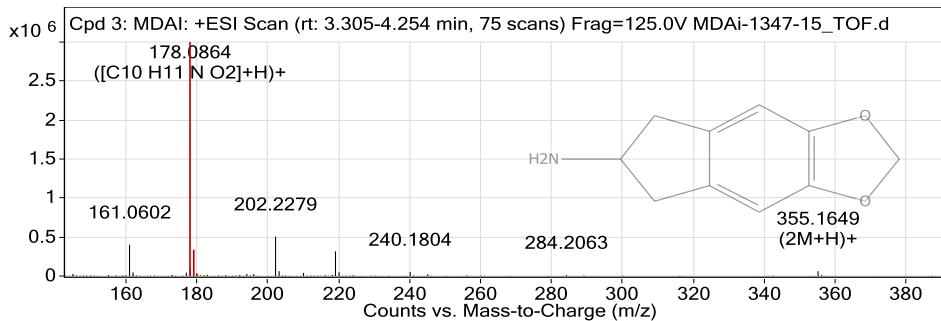

## MS Spectrum Peak List

Obs. m/z	Charge	Abund	Formula	Ion/Isotope
178.0864	1	3002021.75	C10 H11 N O2	(M+H)+
179.0904	1	327303.58	C10 H11 N O2	(M+H)+
180.092	1	32456.95	C10 H11 N O2	(M+H)+
181.0949	1	2168.97	C10 H11 N O2	(M+H)+
355.1652	1	70127.35		(2M+H)+
356.1682	1	15537.57		(2M+H)+
357.1571	1	3107.72		(2M+H)+
358.1517	1	242.69		(2M+H)+

--- End Of Report ---

### Peak Integration Report

Sample Name:	MDAi_1347-15_IC	Inj. Vol.:	25,00
Injection Type:	Unknown	Dilution Factor:	1,0000
Program:	ANIONI	Operator:	kemija
Inj. Date / Time:	17-nov-2015 / 10:32	Run Time:	42,00

No.	Time min	Peak Name	Peak Type	Area $\mu\text{S}\cdot\text{min}$	Height $\mu\text{S}$	Amount mg/L
1,00	9,24	Chloride	BMB	2,12	8,89	n.a.
TOTAL:				2,12	8,89	0,00

