




## ANALYTICAL REPORT

### MDAI (C<sub>10</sub>H<sub>11</sub>NO<sub>2</sub>)

#### 2H,5H,6H,7H-indeno[5,6-d][1,3]dioxol-6-amine

Remark – other active cpd. detected: **none**

Sample ID:	1597-16
Sample description:	powder - off white
Sample type:	RM-reference material
Comments <sup>1</sup> :	LCG Lot#26113; RESPONSE -purchasing
Date of entry:	7/18/2016

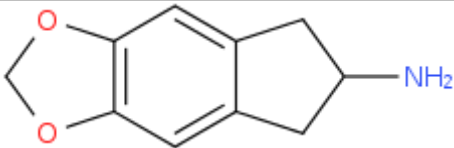Substance identified-structure <sup>2</sup> (base form)	
Systematic name:	2H,5H,6H,7H-indeno[5,6-d][1,3]dioxol-6-amine
Other names:	5,6-methylenedioxy-2-aminoindane; 6,7-dihydro-5H-cyclopenta[f] [1,3]benzodioxol-6-amine
Formula (per base form)	C <sub>10</sub> H <sub>11</sub> NO <sub>2</sub>
M <sub>w</sub> (g/mol)	177.2
Salt form:	base
StdInChIKey	FQDRMHHCWZAXJM-UHFFFAOYSA-N
Compound Class	Aminoindanes
Other active cpd. detected	none
Add.info (purity..)	99,8 %

<sup>1</sup> This report has been produced with the financial support of the Prevention of and fight against crime Programme of the European Union (grant agreement number JUST/2013/ISEC/DRUGS/AG/6413). The contents of this report are the sole responsibility of the National Forensic Laboratory and can in no way be taken to reflect the views of the European Commission.

<sup>2</sup> Created by OPSIN free tool: <http://opsin.ch.cam.ac.uk/> DOI: 10.1021/ci100384d



## Report updates

date	comments (explanation)

## Supporting information

Analytical technique:	applied	remarks
GC-MS (EI ionization)	+	NFL GC-RT (min): 4.33 BP(1): 160; BP(2): 149, BP(3) :177,
FTIR-ATR	+	direct measurement
GC-IR (condensed phase)	+	always as base form

**1. GC-MS (Agilent):** GC-method is RT locked to tetracosane (9.258 min). Injection volume 1 ml and split mode (1:50). Injector temperature: 280 °C. Chromatographic separation: on column HP1-MS (100% dimethylpolysiloxane), length 30 m, internal diameter 0.25 mm, film thickness 0.25 µm. Carrier gas He: flow-rate 1.2 ml/min. GC oven program: 170 °C for 1 min, followed by heating up to 190 °C at rate 8 °C/min, then heating up to 293 °C at a rate of 18 °C/min, hold for 6.1 min, then heating at 50 °C/min up to 325 °C and finally 6.1 min isothermal. MSD source EI = 70 eV. GC-MS transfer line T= 235 °C, source and quadrupole temperatures 280 °C and 180 °C, respectively. Scan range m/z scan range: from 50 (30 until 6 min.) to 550 (300 until 6 min) amu.

**2. FTIR-ATR (Perkin Elmer):** scan range 4000-400 cm<sup>-1</sup>; resolution 4cm<sup>-1</sup>

**3. GC- (MS)-IR condensed phase (GC-MS (Agilent) & IR (Spectra analyses-Danny)**


GC-method: Injection volume 1 ml and split mode (1:5). Injector temperature 280 °C. Chromatographic separation as above (1). Split MS : IR = 1 : 9.

MSD source EI = 70 eV. GC-MS transfer line T= 235 °C, source and quadrupole temperatures 280 °C and 180 °C, respectively. Scan range m/z scan range: from 50 (30 until 6 min.) to 550 (300) amu.


IR (condensed (solid) phase): IR scan range 4000 to 650, resolution 4 cm<sup>-1</sup>.

# FIGURES OF SPECTRA

MS (EI)

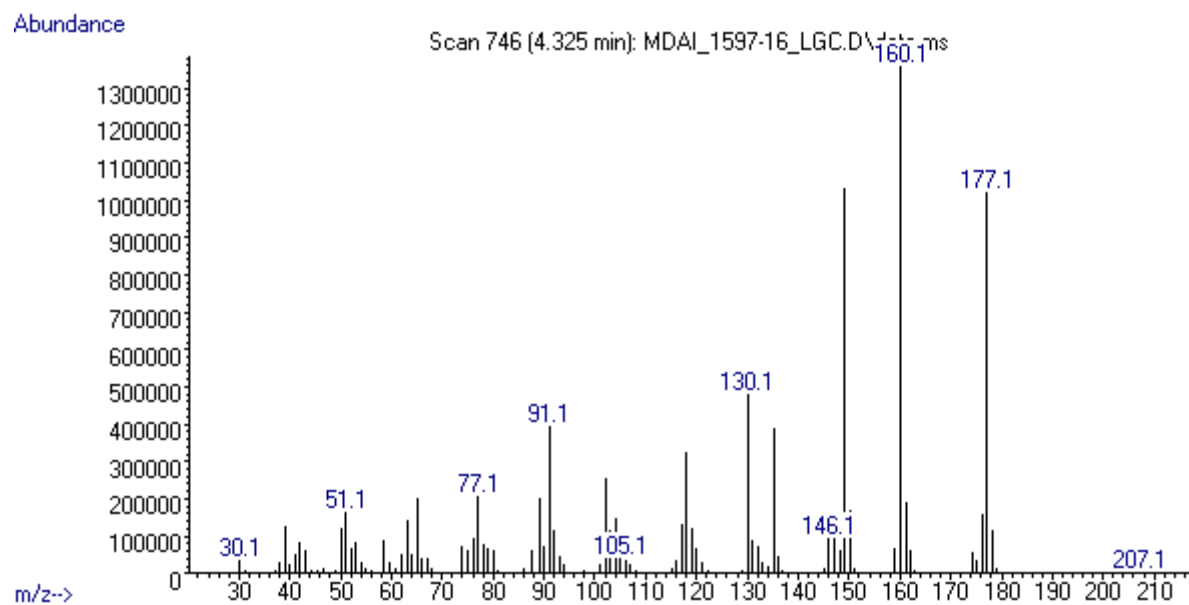


FTIR-ATR

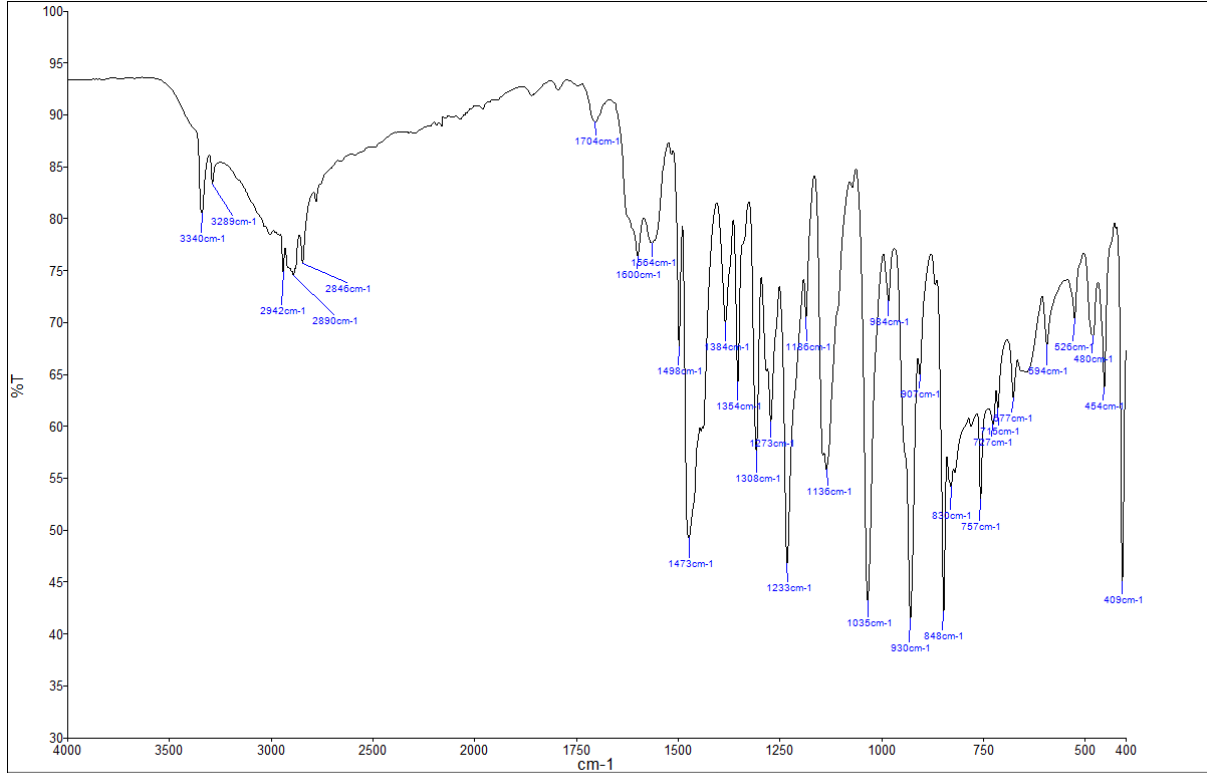

Name	Description
MDAL1597-16-LGC_IR-A	ID: 1597-16; 6,7-dihydro-5H-cyclopenta[f][1,3]benzodioxol-6-amine_Lot#26113

IR-Condensed phase

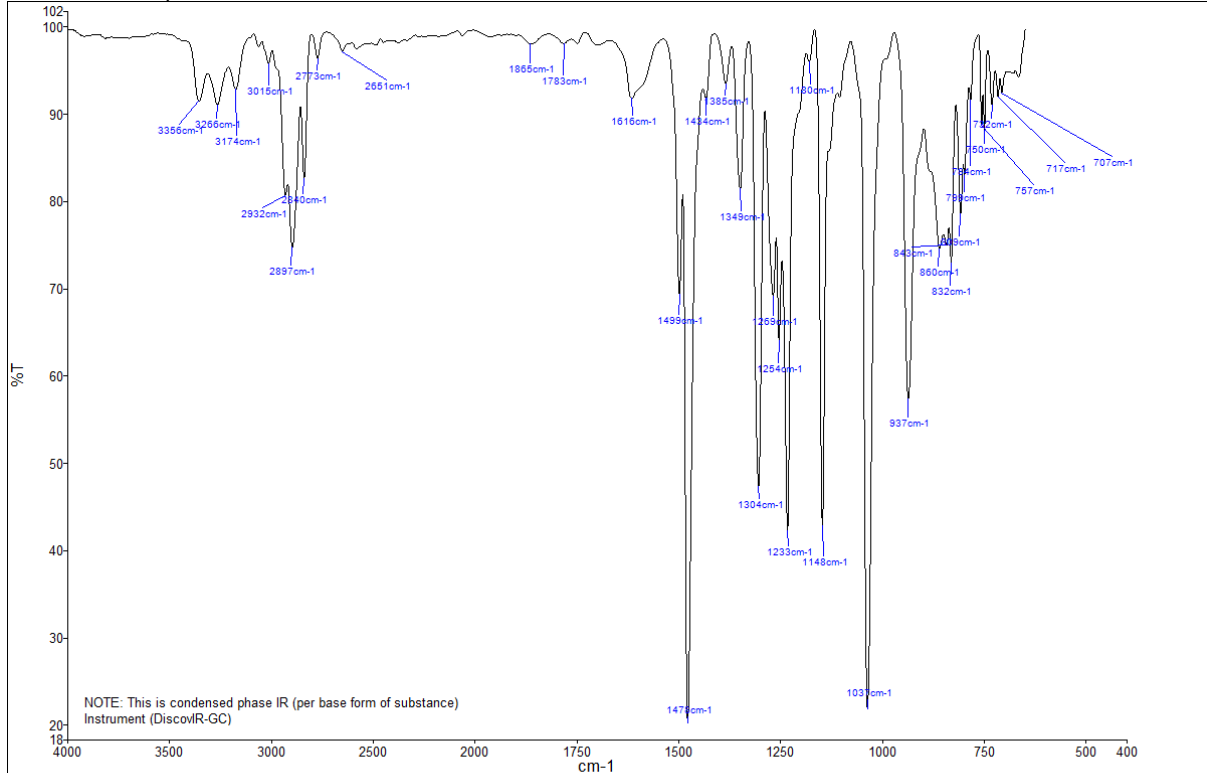

NOTE: This is condensed phase IR (per base form of substance)  
Instrument (DiscovIR-GC)

Name	Description
MDAL1597-16_LGC_IR-C.spc	Sample_ID: 1597-16; 6,7-dihydro-5H-cyclopenta[f][1,3]benzodioxol-6-amine_Lot#26113