



## ANALYTICAL REPORT<sup>1</sup>


N-methyl-2AI (

C10H13N)

**N-methyl-2,3-dihydro-1H-inden-2-amine**

Remark – other NPS detected: **none**

Sample ID:	1349-15
Sample description:	crystalinic - off white
Sample type:	test purchase /RESPONSE -purchasing
Date of sample receipt (M/D/Y):	11/6/2015
Date of entry (M/D/Y) into NFL database:	10/25/2015
Report updates (if any) will be published here:	<a href="http://www.policija.si/apps/nfl_response_web/seznam.php">http://www.policija.si/apps/nfl_response_web/seznam.php</a>

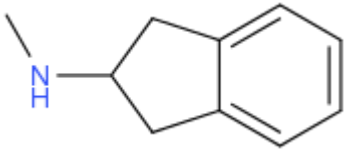Substance identified - structure <sup>2</sup> (base form)	
Systematic name	N-methyl-2,3-dihydro-1H-inden-2-amine
Other names	NM-2AI, N-methyl-2-aminoindane
Formula (per base form)	C10H13N
M <sub>w</sub> (g/mol)	147,22
Salt form	HCl
StdInChIKey	SXWZQUCTTOBHJT-UHFFFAOYSA-N
Compound Class	Aminoindanes
Other NPS detected	none
Add.info (purity..)	impurities not detected

<sup>1</sup> This report has been produced with the financial support of the Prevention of and fight against crime Programme of the European Union (grant agreement number JUST/2013/ISEC/DRUGS/AG/6413). The contents of this report are the sole responsibility of the National Forensic Laboratory and can in no way be taken to reflect the views of the European Commission.

<sup>2</sup> Created by OPSIN free tool: <http://opsin.ch.cam.ac.uk/> DOI: 10.1021/ci100384d

## Report updates

date	comments (explanation)

### Instrumental methods (if applied) in NFL

**1. GC-MS (Agilent):** GC-method is RT locked to tetracosane (RT=9.53 min). Injection volume 1 ml and split mode (1:50) . Injector temperature: 280 °C. Chromatographic separation: on column HP1-MS (100% dimethylpolysiloxane), length 30 m, internal diameter 0.25 mm, film thickness 0.25 mm. Carrier gas He: flow-rate 1.2 ml/min. GC oven program: 170 °C for 1 min, followed by heating up to 293 °C at a rate of 18 °C/min, hold for 6.1 min, then heating at 50 °C/min up to 325 °C and finally 2.8 min isothermal. MSD source EI = 70 eV. GC-MS transfer line T= 235°C, source and quadropole temperatures 280°C and 180°C, respectively. Scan range m/z scan range: from 50 (40) to 550 amu.

**2. HPLC-TOF (Agilent):** 6230B TOF with Agilent 1260 Infinity HPLC with binary pump, column: Zorbax Eclipse XDB-C18, 50 x 4.6 mm, 1.8 micron. Mobile phases (A) 0.1% formic acid and 1mM ammonium formate in water; (B) 0.1% formic acid in methanol (B). Gradient: starting at 5% B, changing to 40% B over 4 min, then to 70% over 2 min and in 5 min to 100%, hold 1 min and back to 5%, equilibration for 1.7 min. The flow rate: 1.0 ml/min; Injection volume 1 µl. MS parameters: 2GHz, Extended Dynamic range mode to a maximum of 1700 amu, acquisition rate 1.30 spectra/sec. Sample ionisation: by Agilent Jet Stream technology (Dual AJS ESI). Ion source: positive ion scan mode with mass scanning from 82 to 1000 amu. Other TOF parameters: drying gas (N<sub>2</sub>) and sheath temperature 325 °C; drying gas flow rate 6 l/min; sheath gas flow rate 8 l/min; nebulizer 25 psig; Vcap. 4000 V; nozzle 2000 V; skimmer 65 V; fragmentor 175 V and Octopole RF 750 V.

**3. FTIR-ATR (Perkin Elmer):** scan range 4000-400 cm<sup>-1</sup>; resolution 4cm<sup>-1</sup>

**4. GC- (MS)-IR condensed phase (GC-MS (Agilent) & IR (Spectra analyses-Danny)**

GC-method: Injection volume 1 ml and split mode (1:5). Injector temperature 280 °C. Chromatographic separation as above (**1**). Split MS : IR = 1:9.

MSD source EI = 70 eV. GC-MS transfer line T= 235°C, source and quadropole temperatures 280°C and 180°C, respectively. Scan range m/z scan range: from 50 (40) to 550 amu.

IR (condensed phase): IR scan range 4000 to 650, resolution 4 cm<sup>-1</sup>.

**5. IC (anions) (Thermo Scientific, Dionex ICS 2100),** Column: IonPac AS19, 2 x 250mm; Eluent: 10mM from 0 to 10 min, 10-58 mM from 10 to 40min; Flow rate: 0.25 ml/min; Temperature: 30°C; Suppressor: AERS 500 2mm, suppressor current 13mA; Inj. Volume: 25 µl

## Supporting information


Solubility in	result/remark
CH <sub>2</sub> Cl <sub>2</sub>	partially
MeOH	soluble
H <sub>2</sub> O	

Analytical technique:	applied	remarks
GC-MS (EI ionization)	+	NFL GC-RT (min): 2,73 BP(1): 147; BP(2): 42,BP(3) :106,
HPLC-TOF	+	Exact mass (theoretical): 147,1048; measured value Δppm:-0,48; formula: C <sub>10</sub> H <sub>13</sub> N
FTIR-ATR	+	direct measurement (sample as received)
FTIR (condensed phase) always as base form		
IC (anions)		
NMR (in FKKT)		no
validation		MS-consistent with 2015ENFSI.L (QM =0.98),
other		


# ANALYTICAL RESULTS

MS (EI)

Abundance

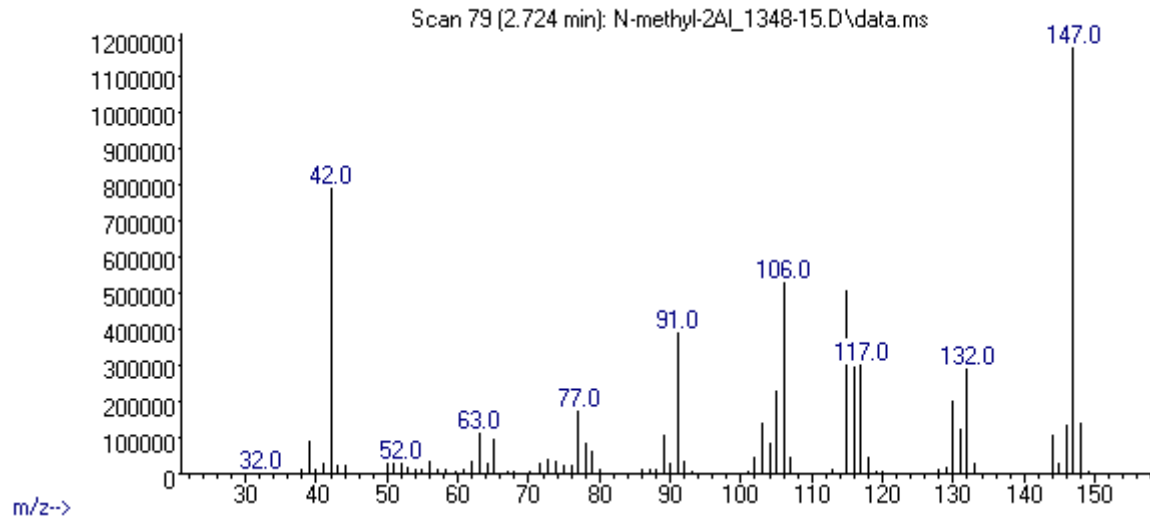

# FTIR-ATR - direct measurement (sample as received)

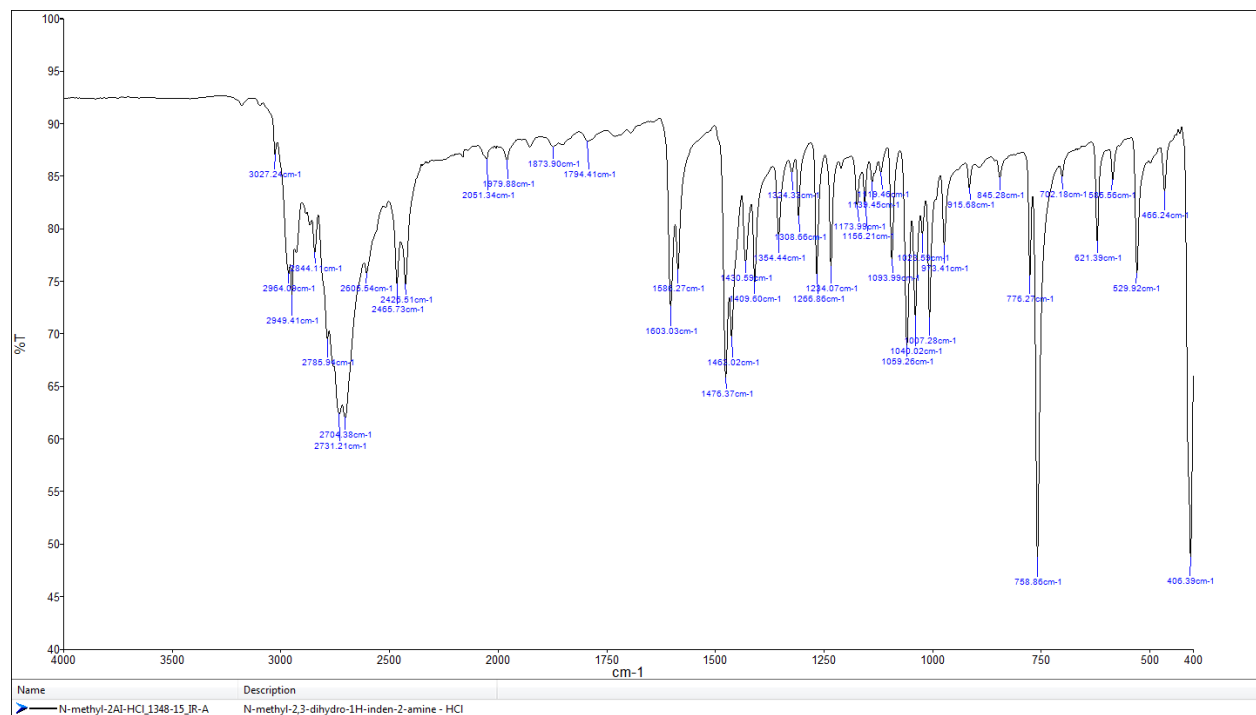

# IR (condensed phase – after chromatographic separation)

# TOF REPORT


<b>Data File</b>	N-Methyl-2AI_1349-15_TOF.d	<b>Sample Name</b>	ID_1349-15
<b>Sample Type</b>	Sample	<b>Position</b>	P1-A4
<b>Instrument Name</b>	6230B TOF LC-MS	<b>User Name</b>	TG
<b>Acq Method</b>	general-17112015-XDB-C18-ESI-poz.m	<b>Acquired Time</b>	11/17/2015 9:59:40 AM
<b>IRM Calibration Status</b>	Success	<b>DA Method</b>	Drugs_NFL.m
<b>Comment</b>	extract in MeOH		

## Compound Table


Label	Compound Name	MFG Formula	Obs. RT	Obs. Mass
Cpd 2: N-methyl-AI	N-methyl-AI	C10 H13 N	3.367	147.1049

Name	Obs. m/z	Obs. RT	Obs. Mass	DB RT	DB Formula	DB Mass	DB Mass Error (ppm)
N-methyl-AI	148.1123	3.367	147.1049	3.37	C10 H13 N	147.1048	-0.48


## Compound Chromatograms

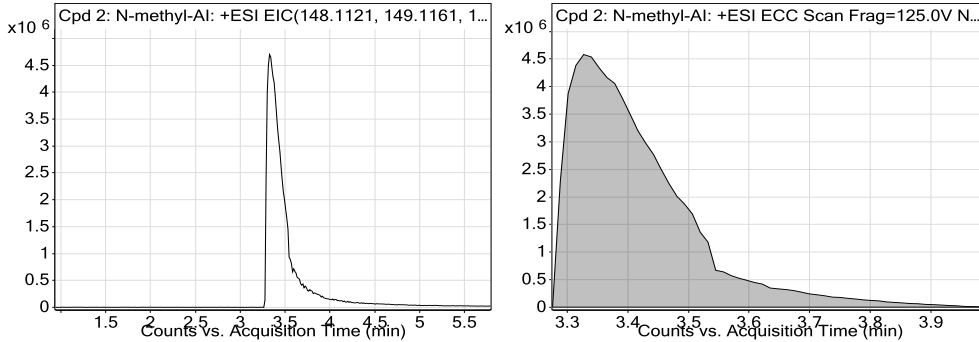

## MFE MS Zoomed Spectrum

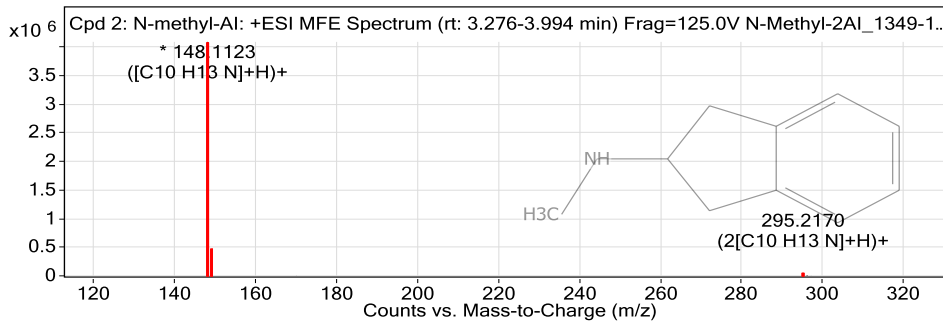

## MS Zoomed Spectrum

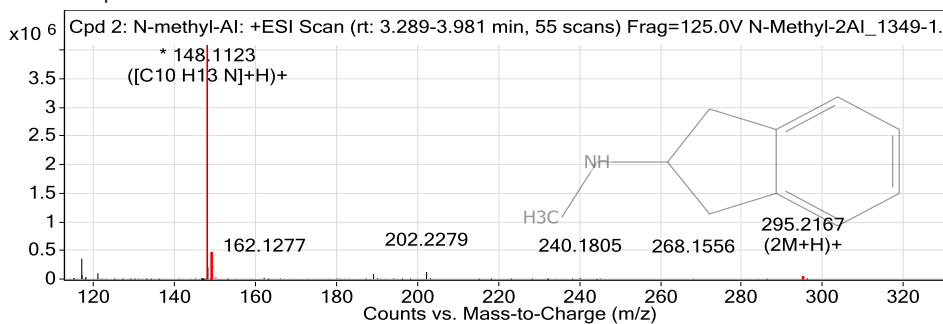

## MS Spectrum Peak List

Obs. m/z	Charge	Abund	Formula	Ion/Isotope
148.1123	1	4086018.75	C10 H13 N	(M+H)+
149.1162	1	441923.58	C10 H13 N	(M+H)+
170.0941	1	1252.49	C10 H13 N	(M+Na)+
295.217	1	46344.61	C10 H13 N	(2M+H)+
296.2199	1	10186.92	C10 H13 N	(2M+H)+
297.2231	1	1048.89	C10 H13 N	(2M+H)+

--- End Of Report ---

### Peak Integration Report

Sample Name:	N-Methyl-2AI_1349-15_IC	Inj. Vol.:	25,00
Injection Type:	Unknown	Dilution Factor:	1,0000
Program:	ANIONI	Operator:	kemija
Inj. Date / Time:	17-nov-2015 / 12:11	Run Time:	42,00

No.	Time min	Peak Name	Peak Type	Area $\mu\text{S}\cdot\text{min}$	Height $\mu\text{S}$	Amount mg/L
1,00	9,23	Chloride	BMB	3,28	14,00	n.a.
TOTAL:				3,28	14,00	0,00

